


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080123\
Data File : BM041215.D
Acq On : 01 Aug 2023 08:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 31 16:29:28 2023

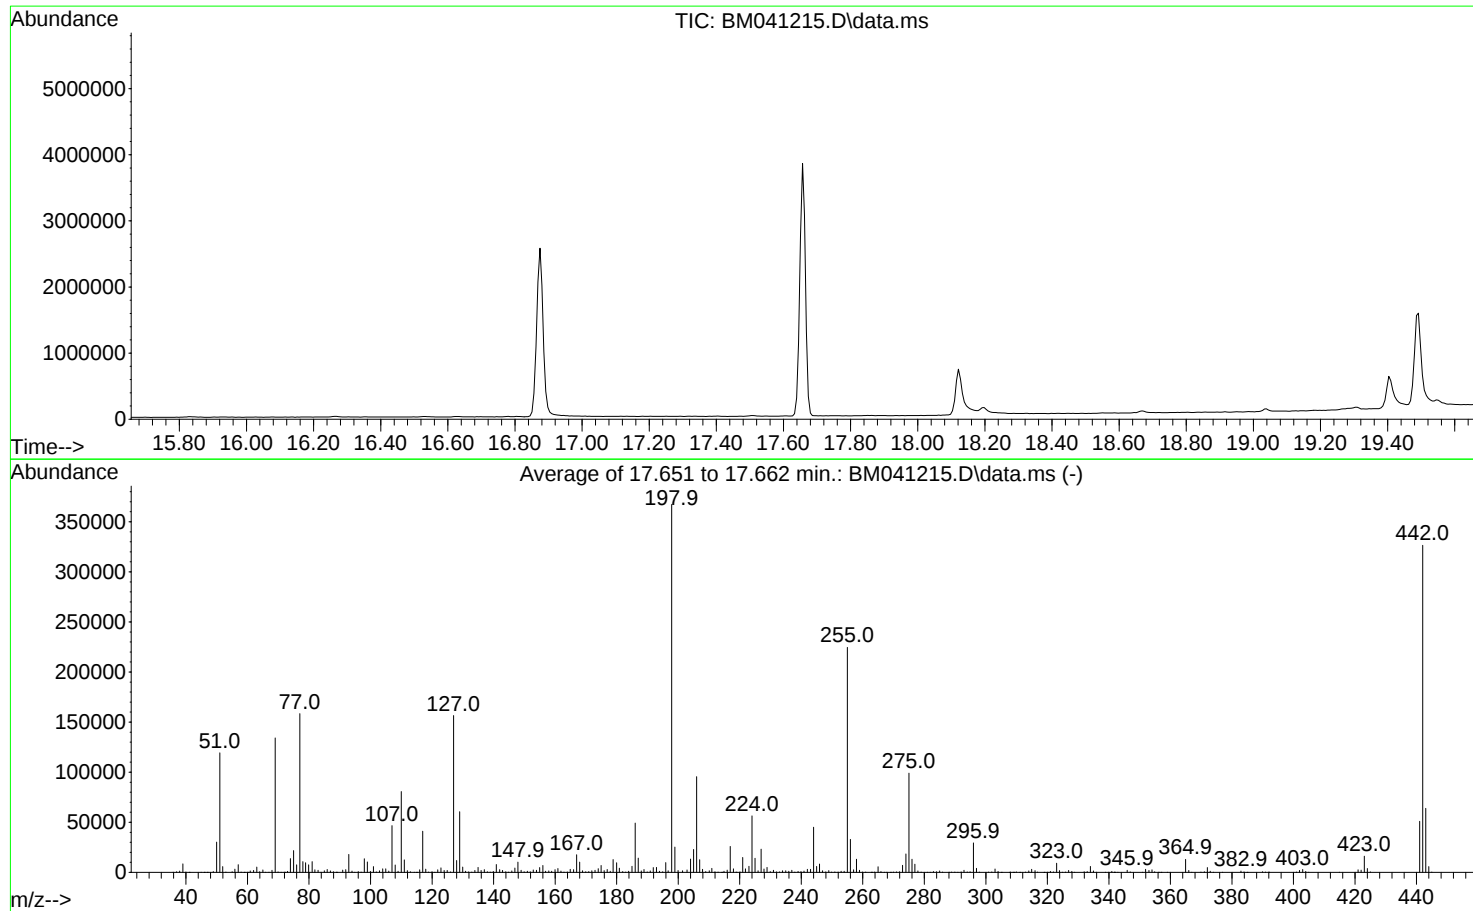

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	119423	PASS
68	69	0.00	2	1.5	2048	PASS
69	198	0.00	100	36.5	134196	PASS
70	69	0.00	2	0.4	520	PASS
127	198	10	80	42.6	156589	PASS
197	198	0.00	2	0.4	1559	PASS
198	198	100	100	100.0	367275	PASS
199	198	5	9	6.9	25275	PASS
275	198	10	60	27.0	98984	PASS
365	198	1	100	3.5	13033	PASS
441	198	0.01	100	13.9	50907	PASS
442	442	50	100	100.0	326528	PASS
443	442	15	24	19.6	63960	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2023	BNA_M	<u>BM041215.D</u>
Compound Name	Response	Retention Time
DDT	1220610	20.715
DDD	25950	20.321
DDE	1616	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27566	1248176	2.21

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080123\
Data File : BM041215.D
Acq On : 01 Aug 2023 08:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 02 04:28:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

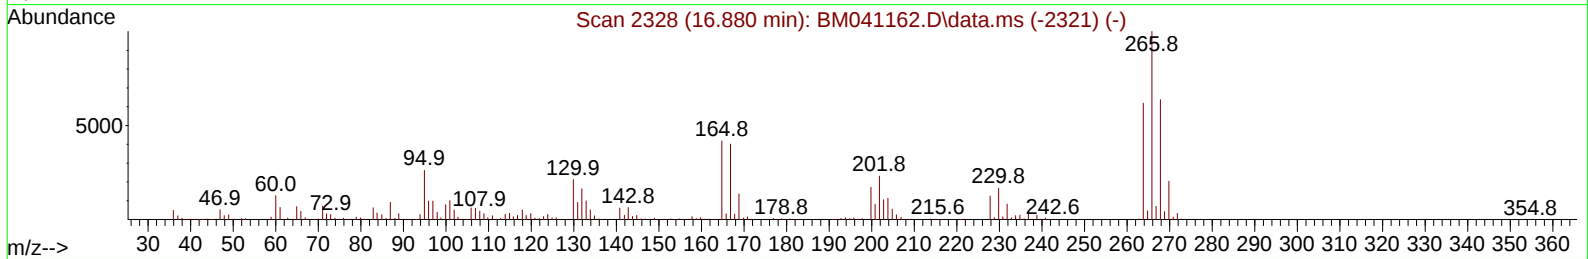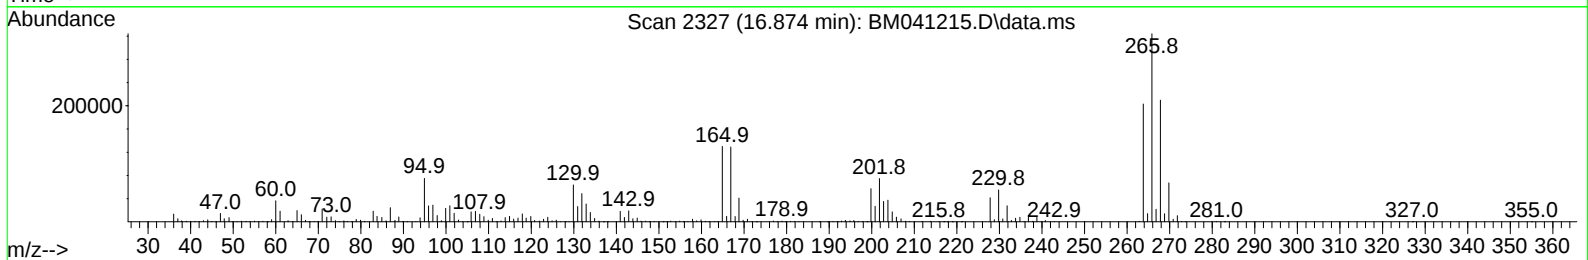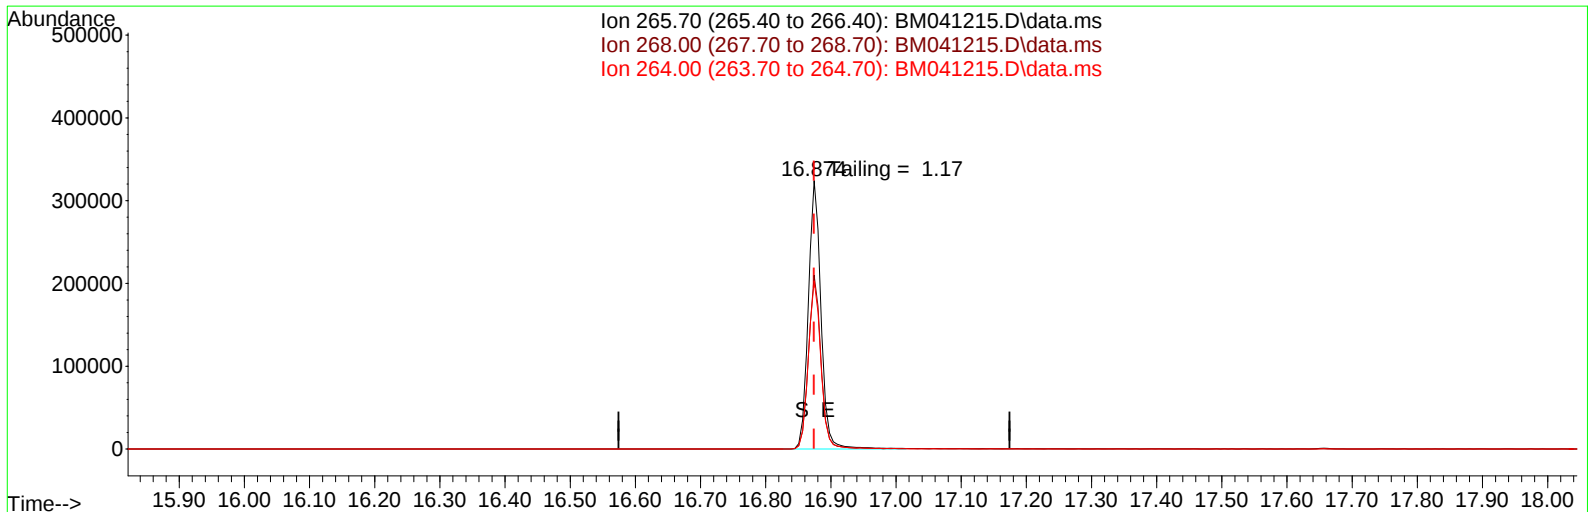

TIC: BM041215.D\data.ms

(70) Pentachlorophenol (C)

16.874min (+ 0.000) 0.00 ng

response 439775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.69
264.00	61.80	62.69
0.00	0.00	0.00

