

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080218\
 Data File : BM016168.D
 Acq On : 02 Aug 2018 23:17
 Operator : SJ/JU
 Sample : J4171-08
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JJ1K1

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:56:11 PM

Quant Time: Aug 03 02:13:38 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 03 01:12:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.19	152	58453	20.00	ng/ul	0.00
18) Naphthalene-d8	11.01	136	247413	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.82	164	121575	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.54	188	231523	20.00	ng/ul	0.00
77) Chrysene-d12	21.67	240	203924	20.00	ng/ul	0.00
85) Perylene-d12	24.03	264	206883	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.45	96	7246	5.46	ng/uL	0.00
5) Phenol-d5	7.35	99	124760	23.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.51	67	85117	25.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.72	132	115978	26.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.90	113	95864	20.96	ng/ul	0.00
19) Nitrobenzene-d5	9.37	128	53229	29.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.09	143	59801	29.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.63	165	102369	26.17	ng/ul	0.00
29) 4-Chloroaniline-d4	11.16	131	106781	22.44	ng/ul	0.00
43) Dimethylphthalate-d6	14.22	166	311105	28.07	ng/ul	0.00
46) Acenaphthylene-d8	14.52	160	344018	27.22	ng/ul	0.00
51) 4-Nitrophenol-d4	15.05	143	28040m	14.60	ng/ul	0.00
57) Fluorene-d10	15.80	176	246390	26.21	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.95	200	24659	15.96	ng/ul	0.00
70) Anthracene-d10	17.64	188	328242	27.69	ng/ul	0.00
78) Pyrene-d10	19.91	212	329600	34.87	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.87	264	330951	29.09	ng/ul	0.00

Target Compounds				Ovalue	
44) Dimethylphthalate	14.27	163	28203	2.570	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080218\
Data File : BM016168.D
Acq On : 02 Aug 2018 23:17
Operator : SJ/JU
Sample : J4171-08
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JJ1K1

Manual Integrations
APPROVED

Sohil
8/3/2018 5:56:11 PM

Quant Time: Aug 03 02:13:38 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM071318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 03 01:12:01 2018
Response via : Initial Calibration

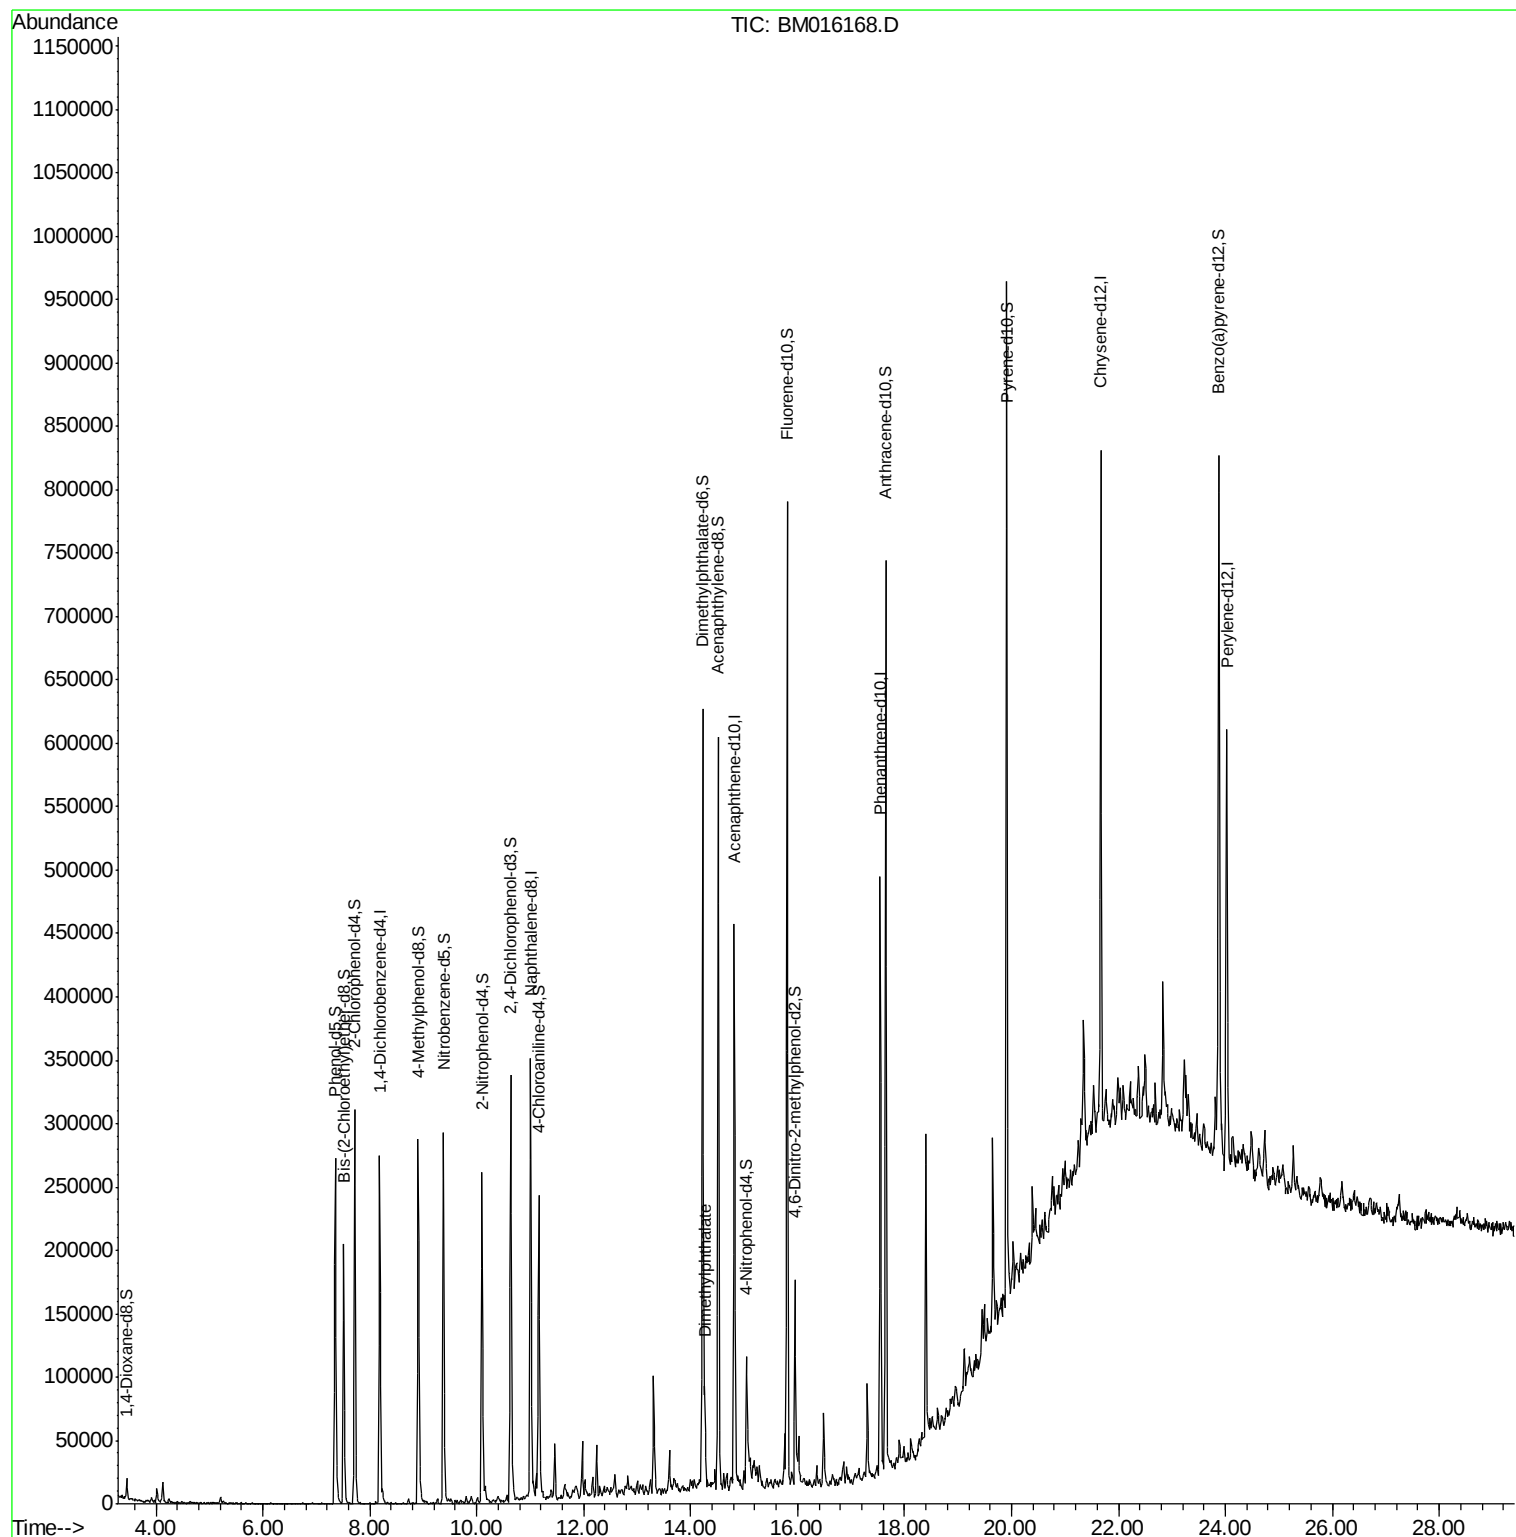

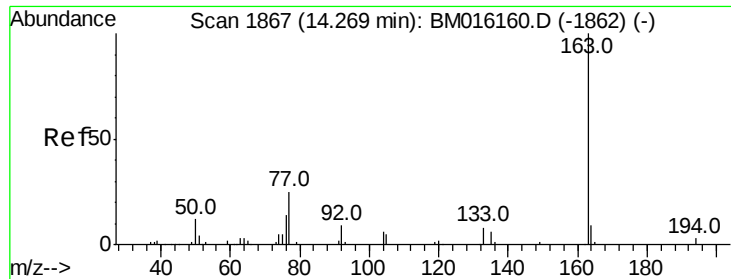

#44
 Dimethylphthalate
 Concen: 2.570 ng/ul
 RT: 14.27 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: BM016168.D
 Acq: 02 Aug 2018 23:17

Instrument :
 BNA_M
 ClientSampleId :
 JJ1K1

Tot Ion	Ratio	Resp	Lower	Upper
163	100	28203		
194	3.7		3.2	4.8
164	9.6		7.8	11.8

Manual Integrations
 APPROVED

Sohil
 8/3/2018 5:56:11 PM

