

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080219\
 Data File : BM021770.D
 Acq On : 02 Aug 2019 23:25
 Operator : HP/JU
 Sample : MDL-W-01
 Misc : 0.07PPM
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 03 06:34:06 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Aug 03 05:33:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	778	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	3488	0.40	ng/ul	0.04
6) Acenaphthene-d10	14.33	164	1747	0.40	ng/ul	0.02
10) Phenanthrene-d10	17.10	188	3037	0.40	ng/ul	0.02
16) Chrysene-d12	21.28	240	2101	0.40	ng/ul	0.01
20) Perylene-d12	23.50	264	2019	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	1648	0.36	ng/ul	0.05
14) Fluoranthene-d10	19.11	212	2496	0.36	ng/ul	0.01


Target Compounds				Ovalue		
3) Naphthalene	10.57	128	721	0.074	ng/ul#	45
5) 2-Methylnaphthalene	12.21	142	399	0.071	ng/ul	97
7) Acenaphthylene	14.06	152	531	0.061	ng/ul#	60
8) Acenaphthene	14.40	153	508	0.068	ng/ul#	90
9) Fluorene	15.42	166	456	0.059	ng/ul#	92
12) Phenanthrene	17.13	178	682	0.067	ng/ul#	72
13) Anthracene	17.25	178	498	0.064	ng/ul#	65
15) Fluoranthene	19.15	202	738	0.073	ng/ul	71
17) Pyrene	19.52	202	752	0.081	ng/ul#	78
18) Benzo(a)anthracene	21.27	228	472	0.075	ng/ul#	80
19) Chrysene	21.32	228	962	0.091	ng/ul#	83
21) Benzo(b)fluoranthene	22.83	252	806	0.090	ng/ul#	39
22) Benzo(k)fluoranthene	22.89	252	801	0.084	ng/ul#	37
23) Benzo(a)pyrene	23.43	252	475	0.067	ng/ul#	17
24) Indeno(1,2,3-cd)pyrene	25.80	276	467	0.057	ng/ul#	33
25) Dibenzo(a,h)anthracene	25.81	278	396	0.062	ng/ul#	7
26) Benzo(a,h,i)perylene	26.46	276	474	0.060	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080219\
Data File : BM021770.D
Acq On : 02 Aug 2019 23:25
Operator : HP/JU
Sample : MDL-W-01
Misc : 0.07PPM
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 03 06:34:06 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Aug 03 05:33:59 2019
Response via : Initial Calibration




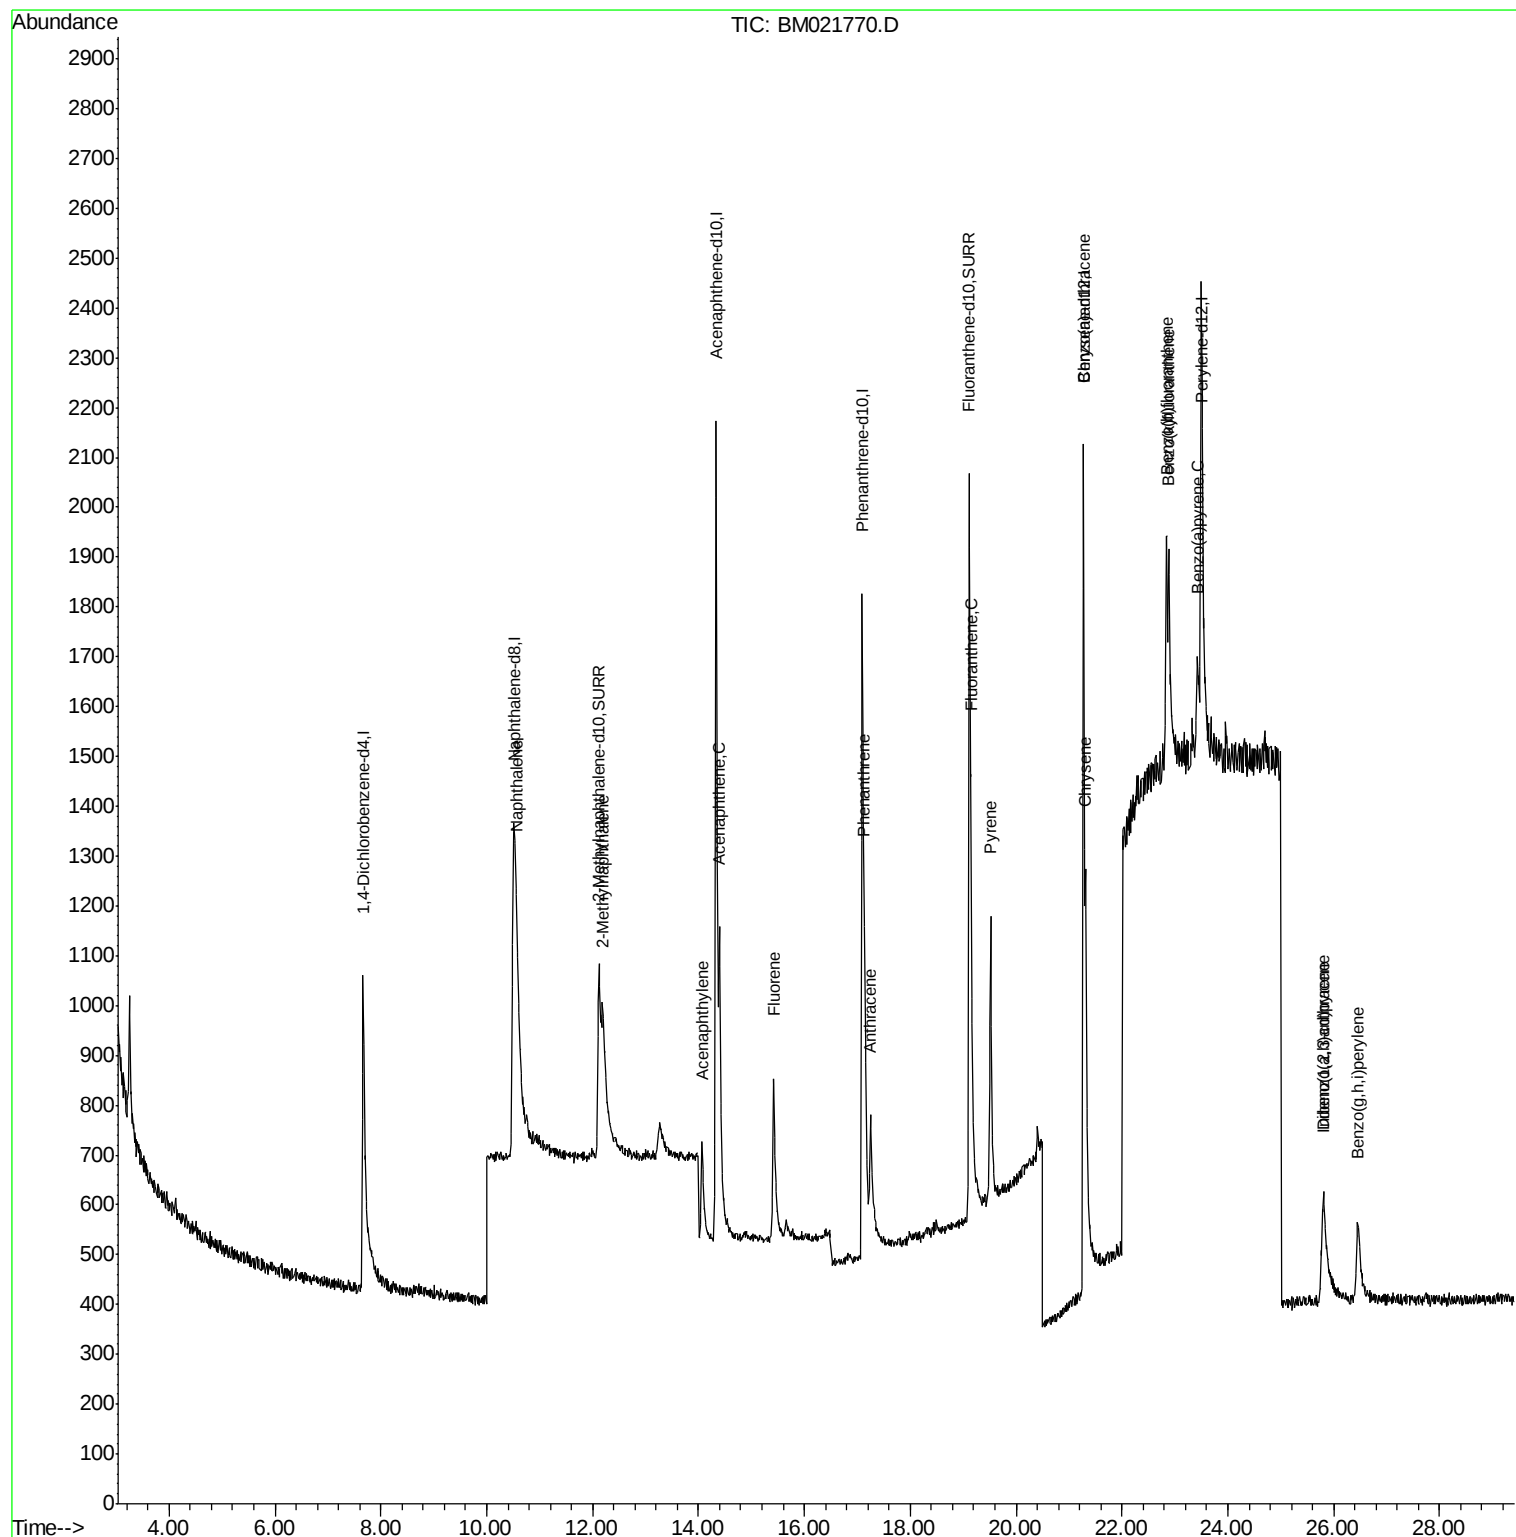




#3
Naphthalene
Concen: 0.074 ng/ul
RT: 10.57 min Scan# 3008
Delta R.T. 0.06 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25




Instrument :
BNA_M
ClientSampleId :


Tot Ion:128 Resp: 721
Ion Ratio Lower Upper
128 100
129 39.1 11.5 17.3#
127 37.9 13.1 19.7#

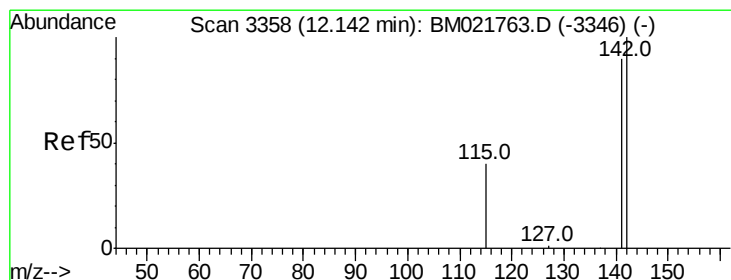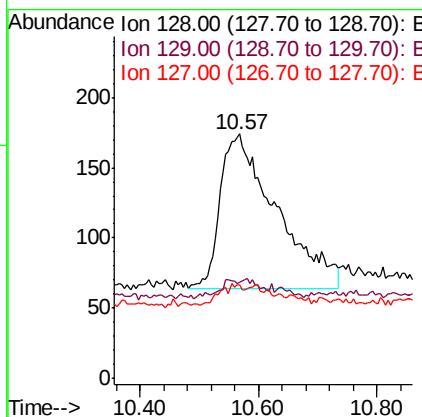

#5
2-Methylnaphthalene
Concen: 0.071 ng/ul
RT: 12.21 min Scan# 3373
Delta R.T. 0.07 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25

Tgt Ion:142 Resp: 399
Ion Ratio Lower Upper
142 100
141 93.0 72.0 108.0

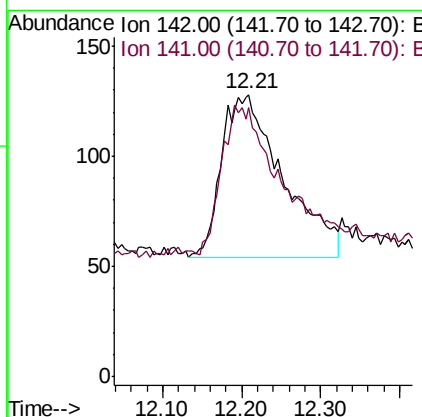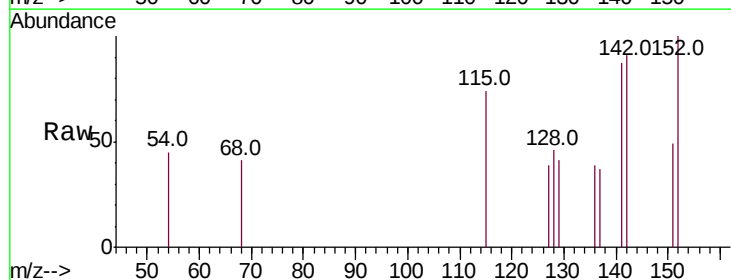



#7

Acenaphthylene

Concen: 0.061 ng/ul

RT: 14.06 min Scan# 3788

Delta R.T. 0.03 min

Lab File: BM021770.D





Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampled :

Tot Ion:	152	Resp:	531
Ion	Ratio	Lower	Upper
152	100		
151	38.0	17.8	26.6#
153	36.6	12.6	18.8#

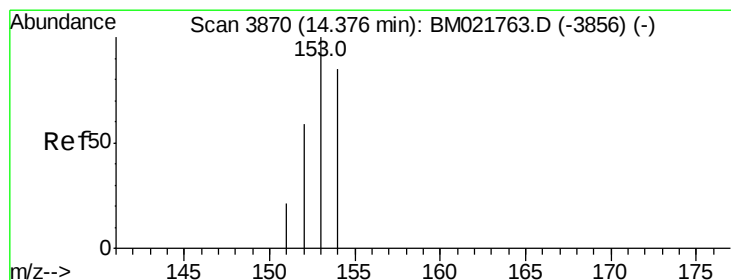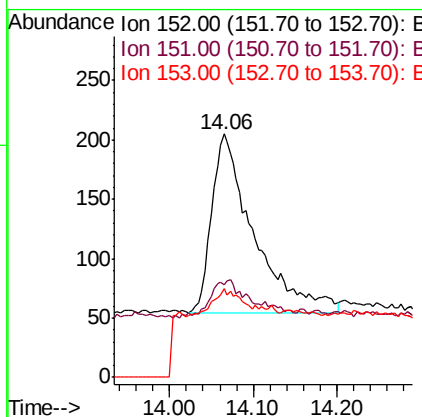

#8

Acenaphthene

Concen: 0.068 ng/ul




RT: 14.40 min Scan# 3876


Delta R.T. 0.02 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Tgt Ion:	153	Resp:	508
Ion	Ratio	Lower	Upper
153	100		
152	66.2	44.0	66.0#
154	91.0	68.0	102.0

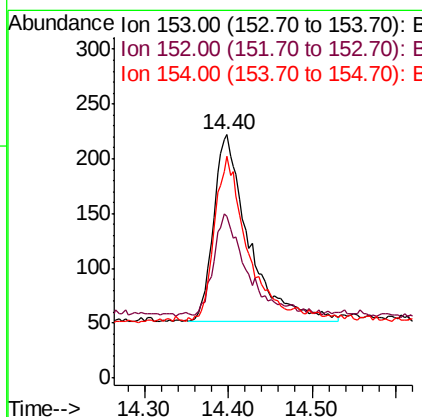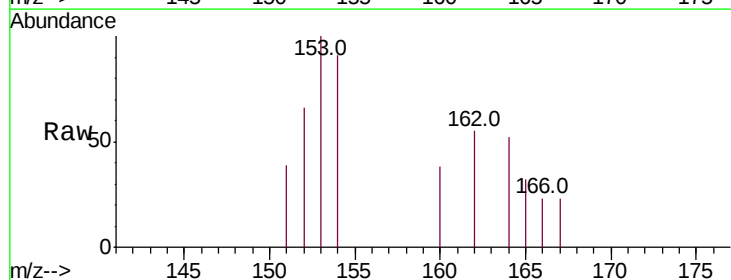



#9

Fluorene

Concen: 0.059 ng/ul

RT: 15.42 min Scan# 4145

Delta R.T. 0.04 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampleId :





Tot Ion:166 Resp: 456

Ion Ratio Lower Upper

166 100

165 102.1 83.0 124.4

167 38.0 13.4 20.2#

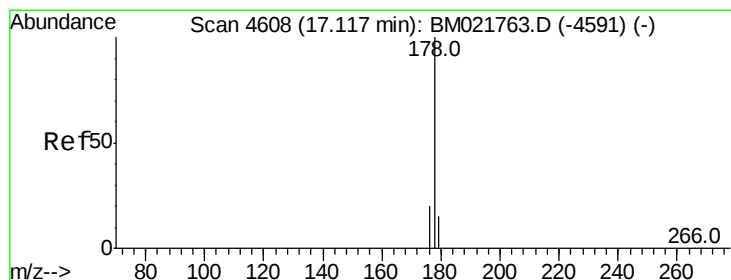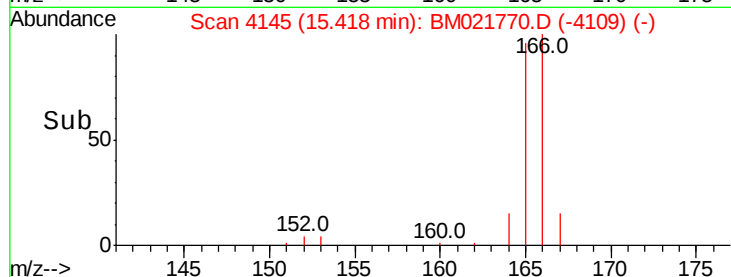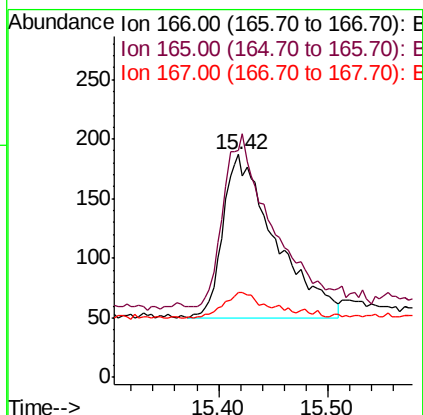

#12

Phenanthrene

Concen: 0.067 ng/ul

RT: 17.13 min Scan# 4613

Delta R.T. 0.02 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25




Tgt Ion:178 Resp: 682


Ion Ratio Lower Upper

178 100

179 32.2 14.0 21.0#

176 32.2 17.0 25.6#

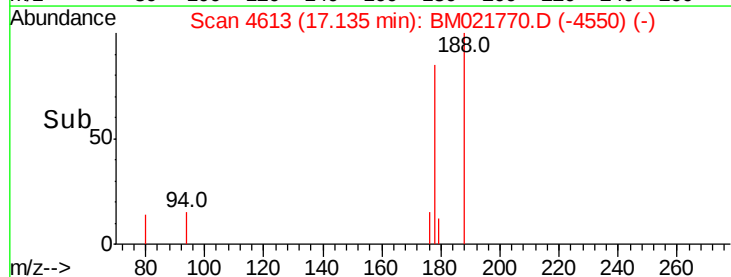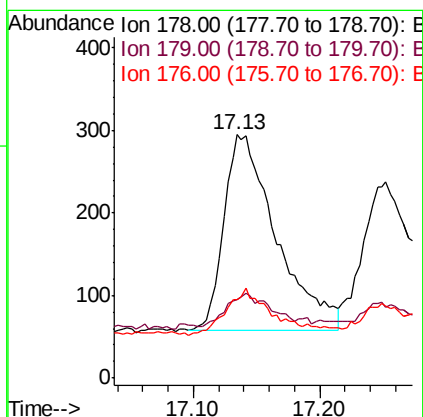

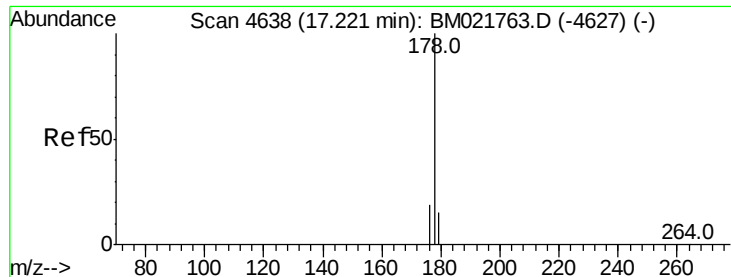

#13

Anthracene

Concen: 0.064 ng/ul

RT: 17.25 min Scan# 4647

Delta R.T. 0.03 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampleId :


Tot Ion:178 Resp: 498

Ion Ratio Lower Upper

178 100

179 35.9 14.5 21.7#




176 37.1 18.1 27.1#

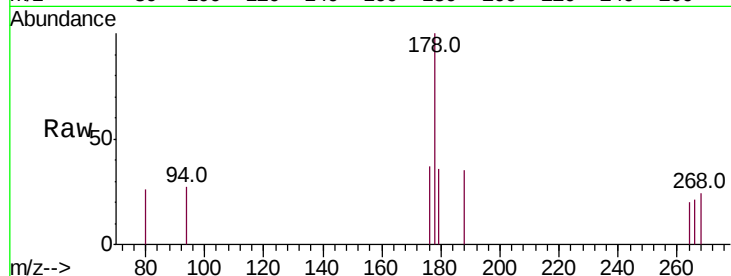

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

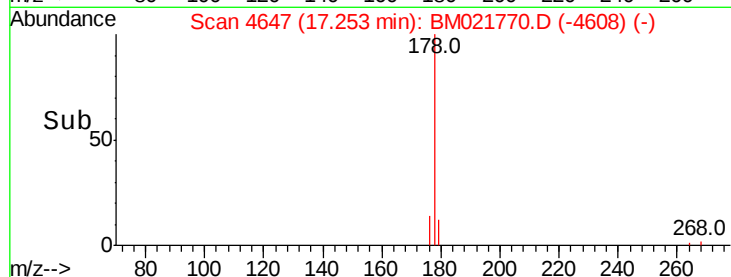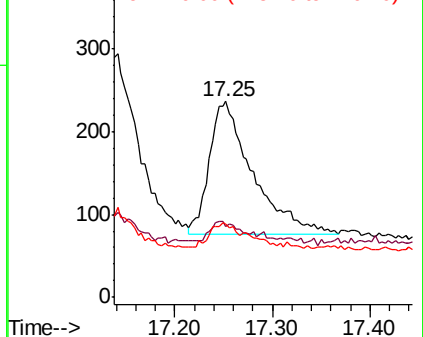

#15

Fluoranthene

Concen: 0.073 ng/ul

RT: 19.15 min Scan# 5176

Delta R.T. 0.02 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25


Tgt Ion:202 Resp: 738

Ion Ratio Lower Upper

202 100

101 31.0 0.0 38.6



100 28.3 0.0 35.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E



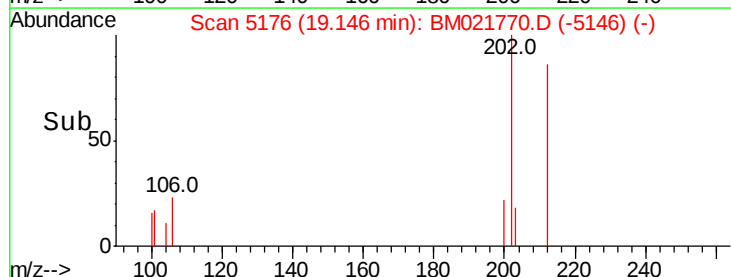
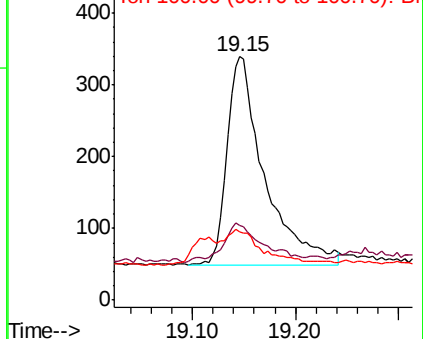




#17
Pvrene
Concen: 0.081 ng/ul
RT: 19.52 min Scan# 5273
Delta R.T. 0.02 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25




Instrument :
BNA_M
ClientSampleId :


Tot Ion:202 Resp: 752
Ion Ratio Lower Upper
202 100
101 31.9 17.0 25.6#
100 27.7 14.3 21.5#

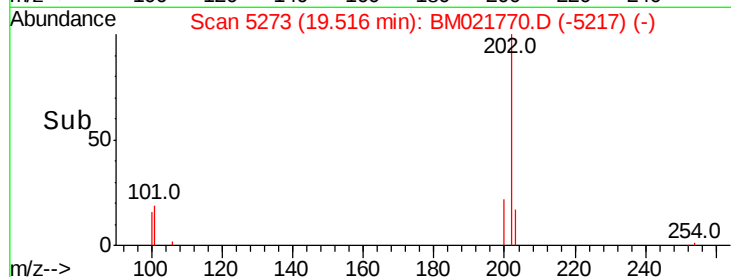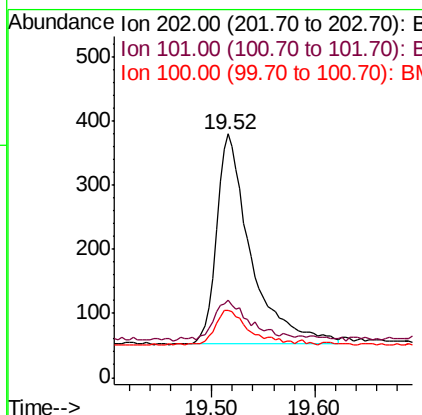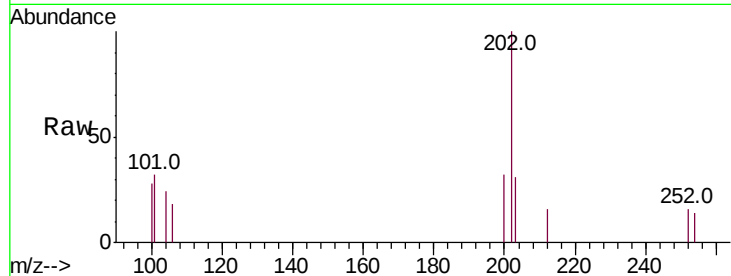

#18
Benzo(a)anthracene
Concen: 0.075 ng/ul
RT: 21.27 min Scan# 5850
Delta R.T. 0.02 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25

Tgt Ion:228 Resp: 472
Ion Ratio Lower Upper
228 100
229 33.0 16.6 24.8#
226 38.5 24.2 36.2#

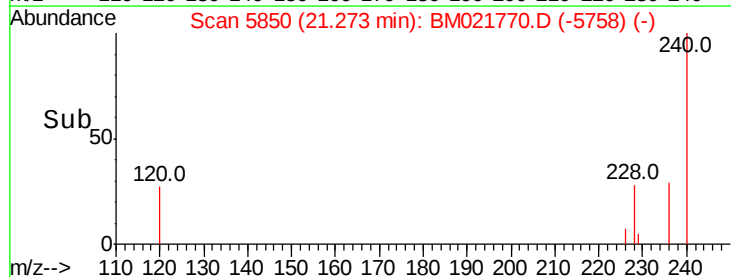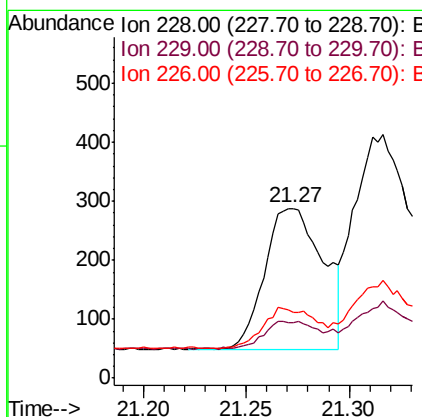



#19

Chrysene

Concen: 0.091 ng/ul

RT: 21.32 min Scan# 5868

Delta R.T. 0.01 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 962

Ion Ratio Lower Upper

228 100

226 40.0 25.6 38.4#




229 32.0 17.6 26.4#



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

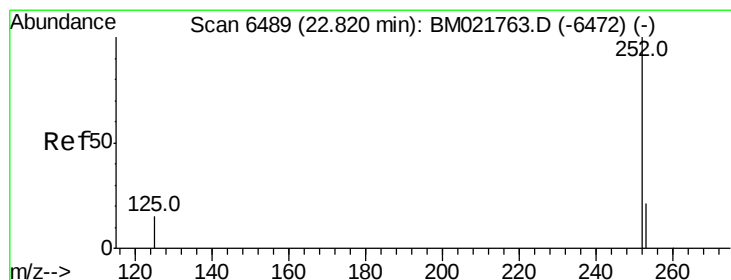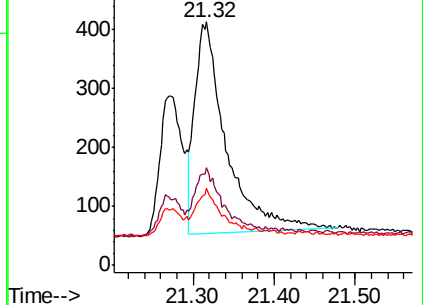

#21

Benzo(b)fluoranthene

Concen: 0.090 ng/ul

RT: 22.83 min Scan# 6495

Delta R.T. 0.01 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25


Tgt Ion:252 Resp: 806

Ion Ratio Lower Upper

252 100

253 61.2 0.0 62.8



125 68.2 0.0 62.2#

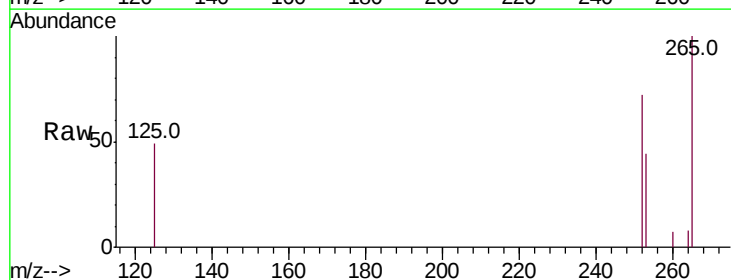


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

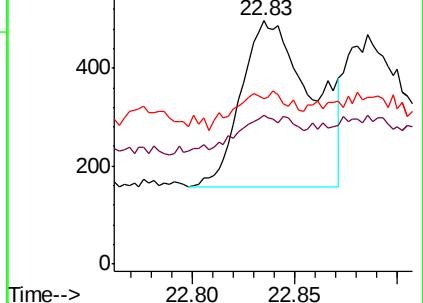

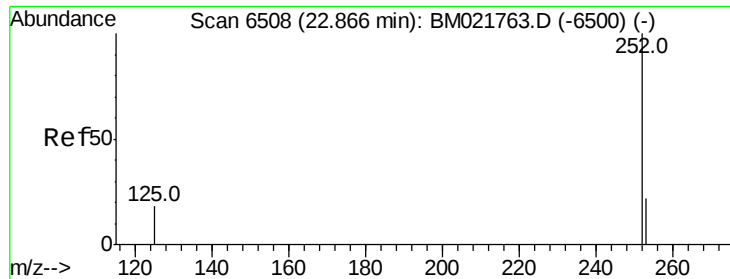

#22

Benzo(k)fluoranthene

Concen: 0.084 ng/ul

RT: 22.89 min Scan# 6516

Delta R.T. 0.02 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampleId :


Tot Ion:252 Resp: 801

Ion Ratio Lower Upper

252 100

253 64.6 25.8 38.8#




125 72.5 27.0 40.4#

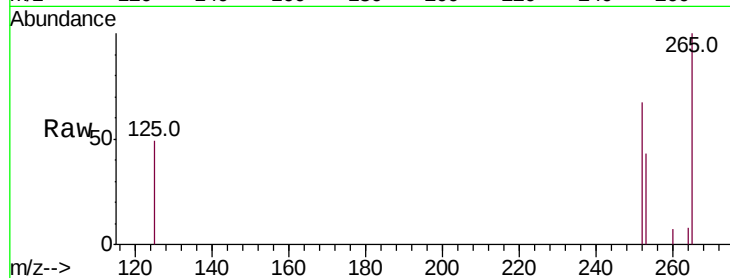

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

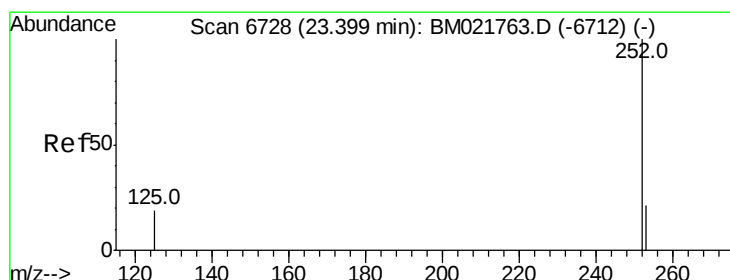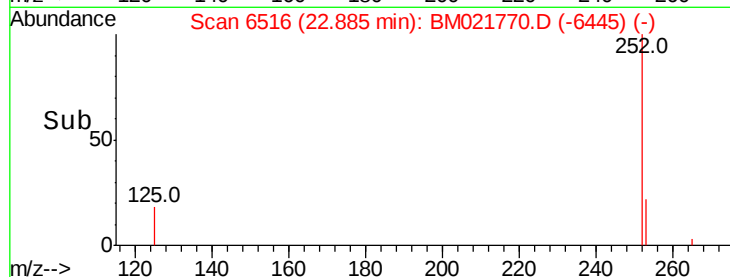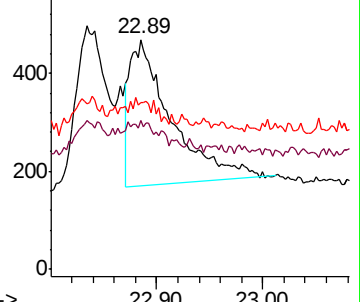

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.43 min Scan# 6741

Delta R.T. 0.03 min

Lab File: BM021770.D

Acq: 02 Aug 2019 23:25


Tgt Ion:252 Resp: 475

Ion Ratio Lower Upper

252 100

253 90.0 32.4 48.6#



125 101.0 35.9 53.9#

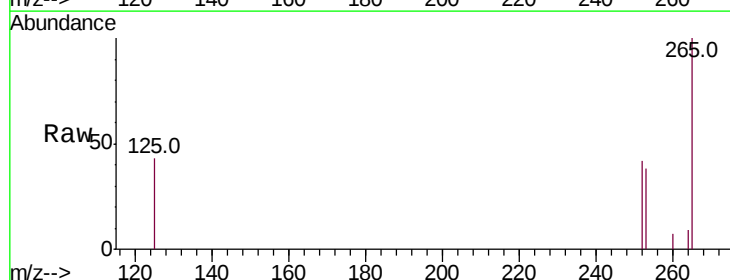


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

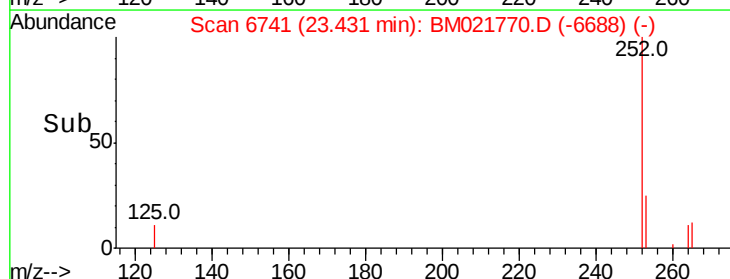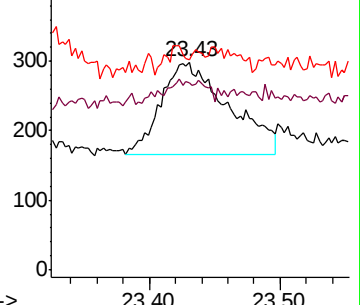







#24

Indeno(1,2,3-cd)pyrene
Concen: 0.057 ng/ul
RT: 25.80 min Scan# 7717
Delta R.T. 0.07 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25

Instrument :
BNA_M
ClientSampleId :




Tot Ion:276 Resp: 467
Ion Ratio Lower Upper
276 100
138 0.0 33.8 50.8#
227 0.0 0.0 0.0

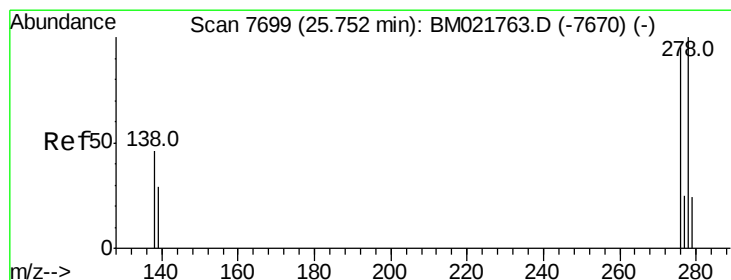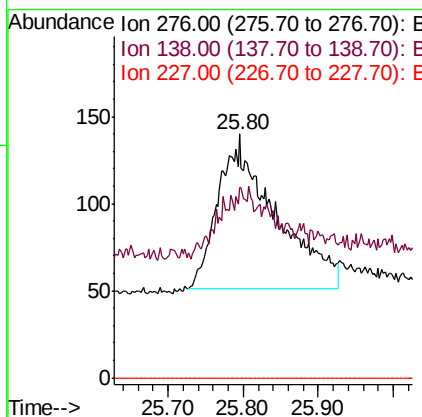


#25

Dibenzo(a,h)anthracene
Concen: 0.062 ng/ul
RT: 25.81 min Scan# 7722
Delta R.T. 0.06 min
Lab File: BM021770.D
Acq: 02 Aug 2019 23:25

Tgt Ion:278 Resp: 396
Ion Ratio Lower Upper
278 100
139 79.5 29.5 44.3#
279 108.0 31.1 46.7#

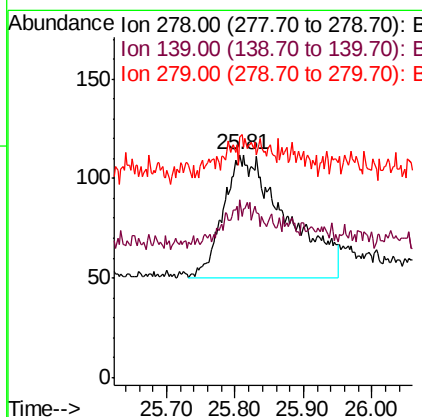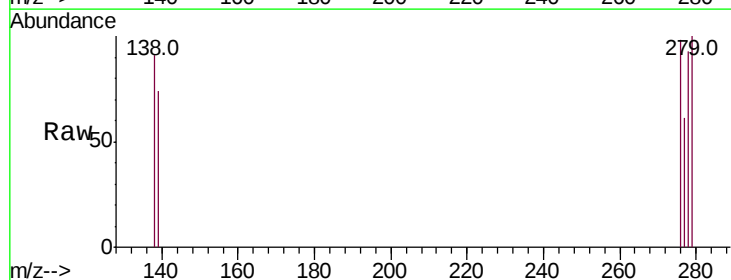

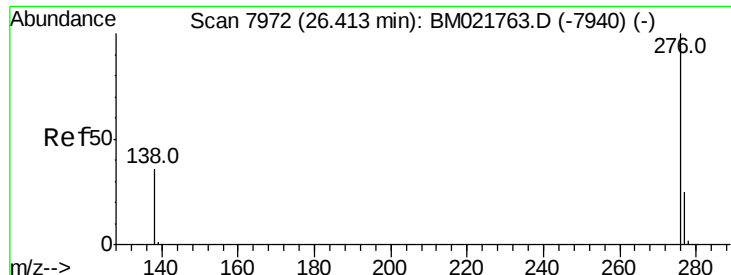

#26

Benzo(a,h,i)perylene

Concen: 0.060 ng/ul

RT: 26.46 min Scan# 7991

Delta R.T. 0.05 min


Lab File: BM021770.D

Acq: 02 Aug 2019 23:25

Instrument :

BNA_M

ClientSampleId :



Tot Ion:276 Resp: 474

Ion Ratio Lower Upper

276 100

138 77.7 36.2 54.2#

277 59.0 24.2 36.2#

