
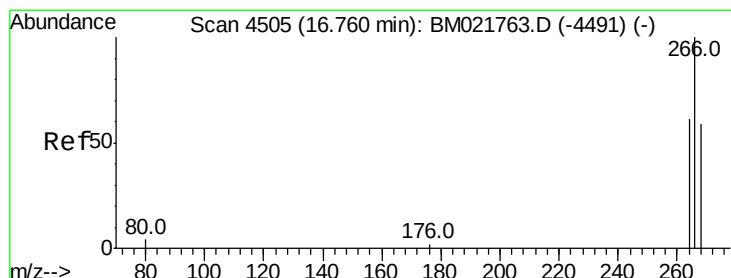
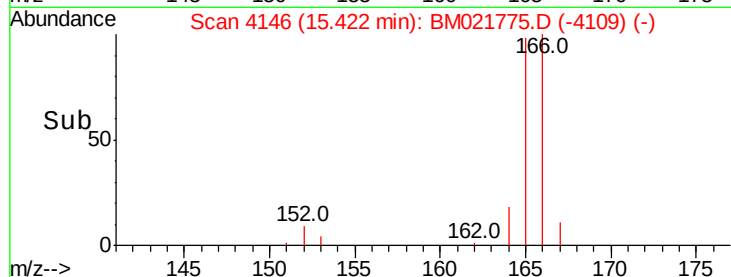
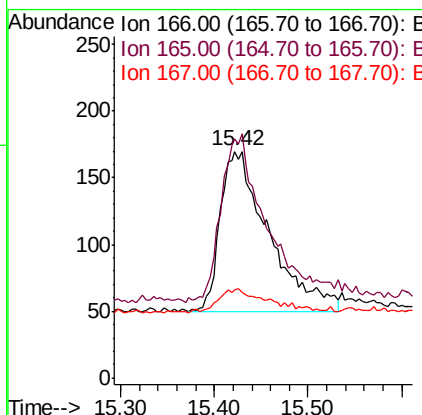


#9
Fluorene
 Concen: 0.063 ng/ul
 RT: 15.42 min Scan# 4146
 Delta R.T. 0.04 min
 Lab File: BM021775.D
 Acq: 03 Aug 2019 04:44

Instrument :
 BNA_M
 ClientSampled :

Tot Ion:166 Resp: 430
 Ion Ratio Lower Upper
 166 100
 165 105.3 83.0 124.4
 167 38.8 13.4 20.2#

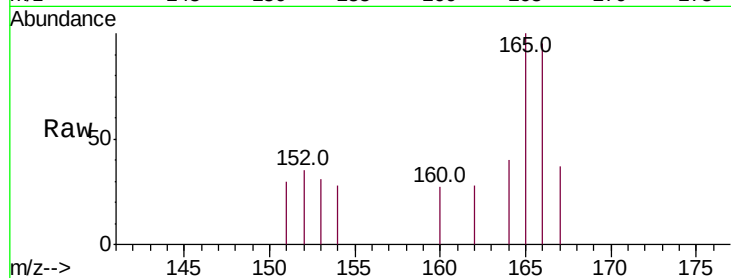

#11
Pentachlorophenol
 Concen: 0.003 ng/ul
 RT: 16.78 min Scan# 4510
 Delta R.T. 0.02 min
 Lab File: BM021775.D
 Acq: 03 Aug 2019 04:44

Tgt Ion:266 Resp: 1
 Ion Ratio Lower Upper
 266 100
 264 0.0 50.9 76.3#
 268 100.0 45.4 68.2#

