
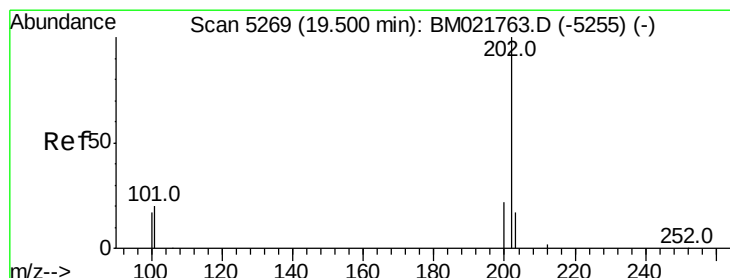
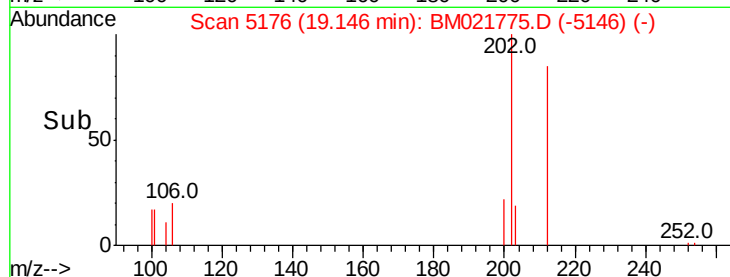
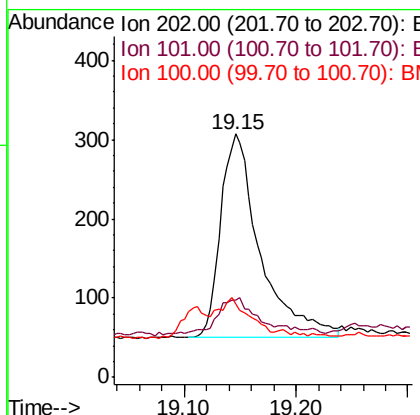


#15
 Fluoranthene
 Concen: 0.072 ng/ul
 RT: 19.15 min Scan# 5176
 Delta R.T. 0.02 min
 Lab File: BM021775.D
 Acq: 03 Aug 2019 04:44

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:202 Resp: 634
 Ion Ratio Lower Upper
 202 100
 101 31.9 0.0 38.6
 100 30.3 0.0 35.6

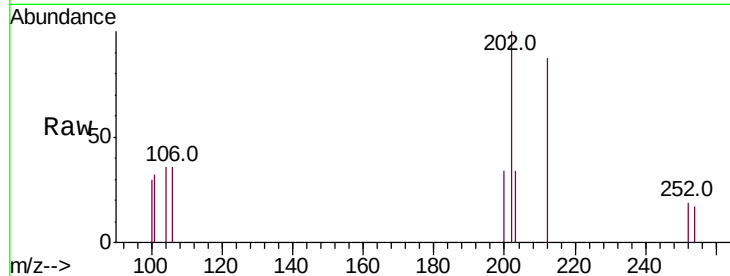

#17
 Pyrene
 Concen: 0.086 ng/ul
 RT: 19.52 min Scan# 5273
 Delta R.T. 0.02 min
 Lab File: BM021775.D
 Acq: 03 Aug 2019 04:44

Tgt Ion:202 Resp: 678
 Ion Ratio Lower Upper
 202 100
 101 34.6 17.0 25.6#
 100 29.6 14.3 21.5#

