

#18

Benzo(a)anthracene

Concen: 0.075 ng/ul

RT: 21.27 min Scan# 5850

Delta R.T. 0.02 min

Lab File: BM021775.D

Acq: 03 Aug 2019 04:44

Instrument :

BNA_M

ClientSampleId :





Tot Ion:228 Resp: 400

Ion Ratio Lower Upper

228 100

229 34.4 16.6 24.8#

226 42.8 24.2 36.2#

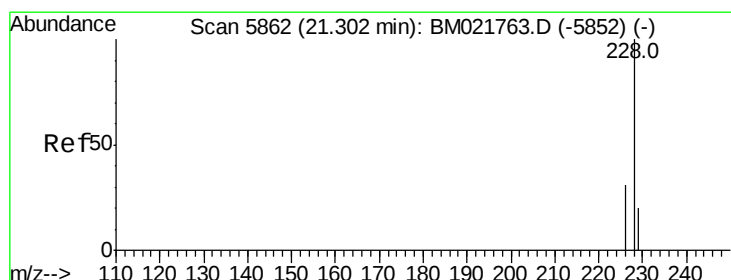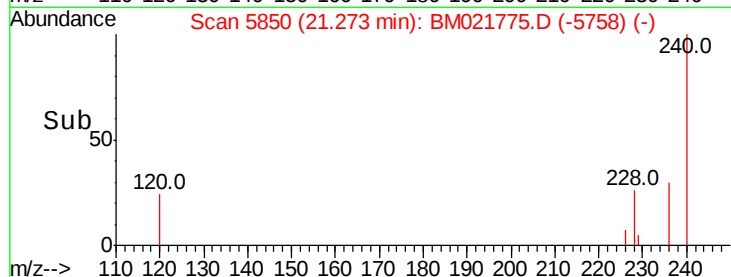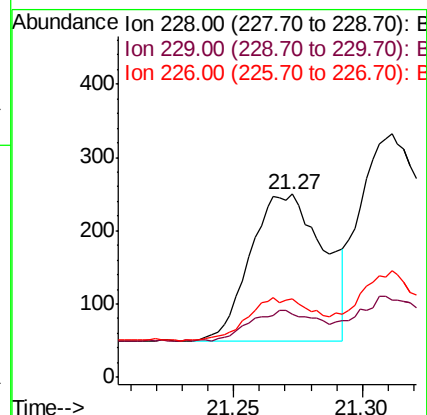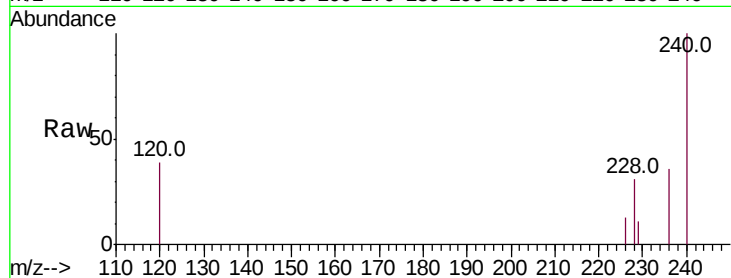

#19

Chrysene

Concen: 0.084 ng/ul

RT: 21.31 min Scan# 5866

Delta R.T. 0.01 min

Lab File: BM021775.D

Acq: 03 Aug 2019 04:44

Tgt Ion:228 Resp: 754

Ion Ratio Lower Upper

228 100

226 43.7 25.6 38.4#

229 31.6 17.6 26.4#

