
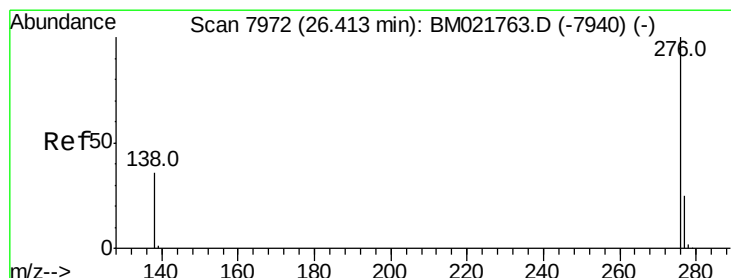
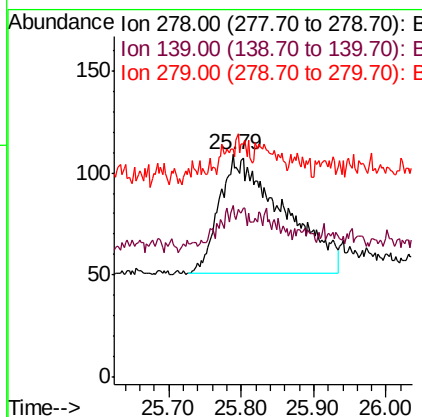
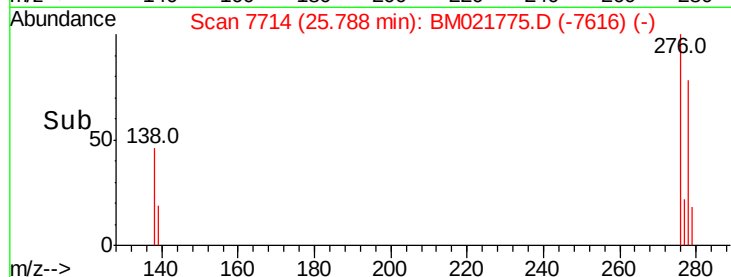


#25
Dibenzo(a,h)anthracene
Concen: 0.061 ng/ul
RT: 25.79 min Scan# 7714
Delta R.T. 0.04 min
Lab File: BM021775.D
Acq: 03 Aug 2019 04:44

Instrument :
BNA_M
ClientSampled :

Tot Ion:278 Resp: 352
Ion Ratio Lower Upper
278 100
139 77.1 29.5 44.3#
279 102.8 31.1 46.7#

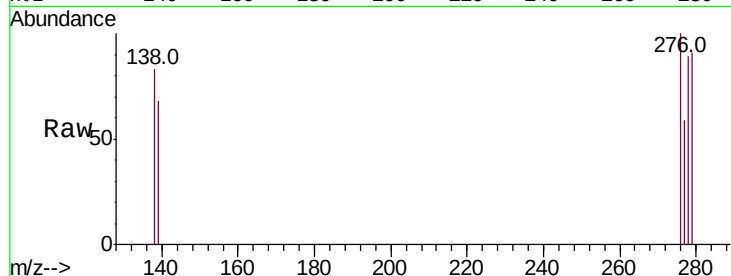

#26
Benzo(g,h,i)perylene
Concen: 0.066 ng/ul
RT: 26.45 min Scan# 7989
Delta R.T. 0.04 min
Lab File: BM021775.D
Acq: 03 Aug 2019 04:44

Tgt Ion:276 Resp: 466
Ion Ratio Lower Upper
276 100
138 70.9 36.2 54.2#
277 59.0 24.2 36.2#

