

#9

Fluorene

Concen: 0.078 ng/ul

RT: 15.42 min Scan# 4145

Delta R.T. 0.04 min

Lab File: BM021774.D

Acq: 03 Aug 2019 04:08

Instrument :

BNA\_M

ClientSampleId :


Tot Ion:166 Resp: 573

Ion Ratio Lower Upper

166 100

165 100.9 83.0 124.4




167 31.0 13.4 20.2#

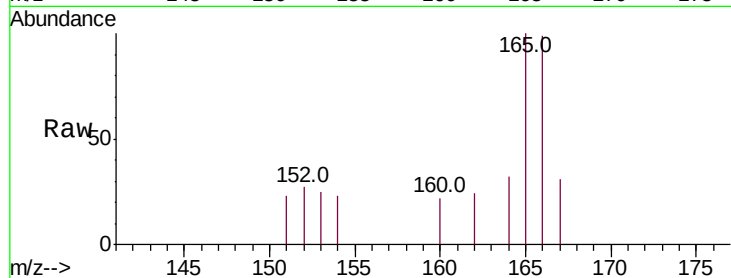

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

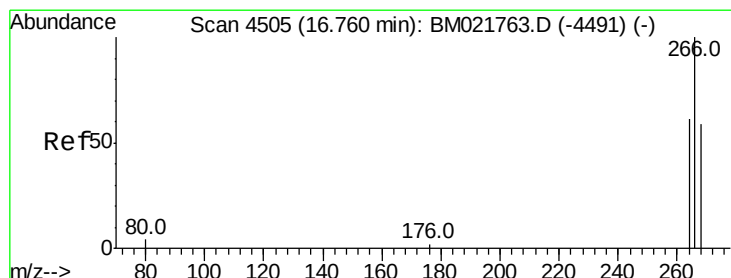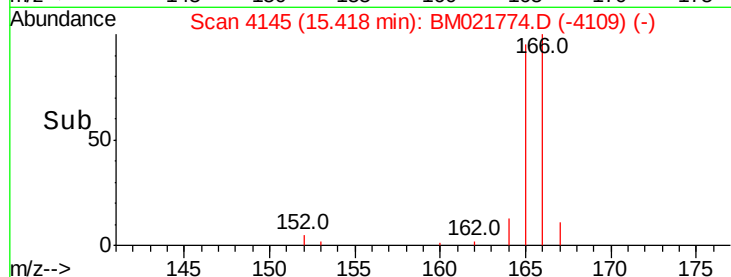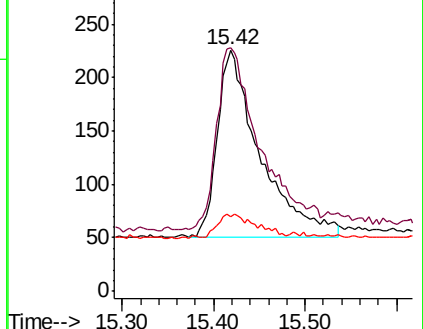

#11

Pentachlorophenol

Concen: 0.002 ng/ul

RT: 16.77 min Scan# 4507

Delta R.T. 0.01 min

Lab File: BM021774.D

Acq: 03 Aug 2019 04:08


Tgt Ion:266 Resp: 1

Ion Ratio Lower Upper

266 100

264 200.0 50.9 76.3#

268 200.0 45.4 68.2#

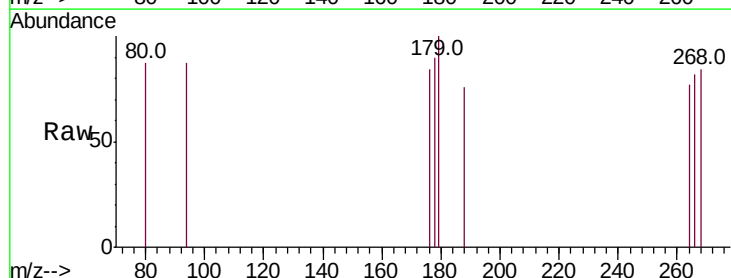

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

