

#18

Benzo(a)anthracene

Concen: 0.089 ng/ul

RT: 21.27 min Scan# 5849

Delta R.T. 0.02 min

Lab File: BM021774.D

Acq: 03 Aug 2019 04:08

Instrument :

BNA_M

ClientSampleId :


Tot Ion:228 Resp: 507

Ion Ratio Lower Upper




228 100

229 32.2 16.6 24.8#

226 38.3 24.2 36.2#

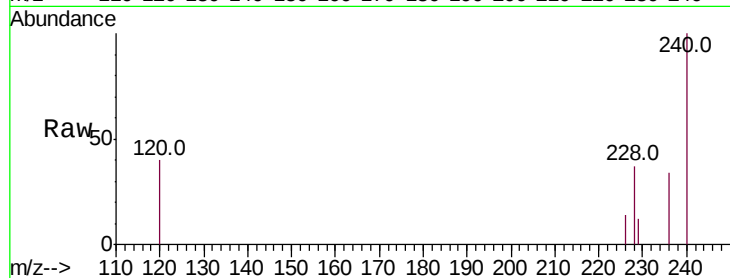

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

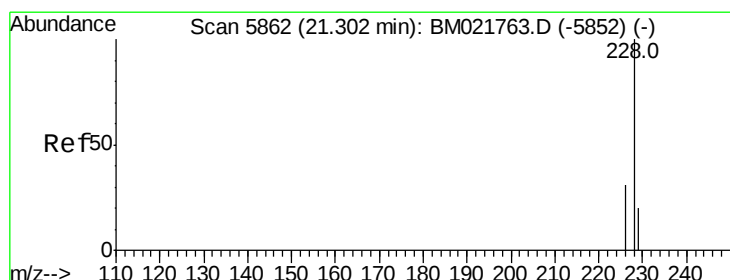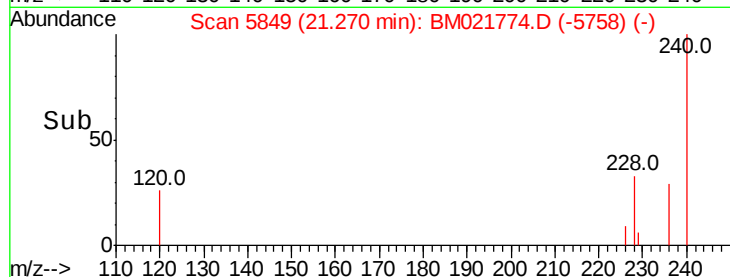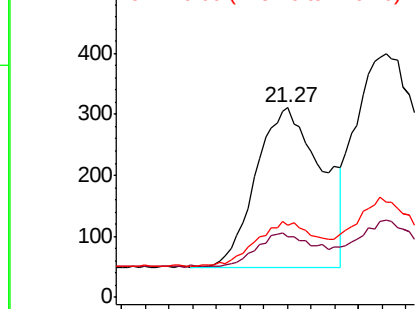

#19

Chrysene

Concen: 0.100 ng/ul

RT: 21.31 min Scan# 5866

Delta R.T. 0.01 min

Lab File: BM021774.D

Acq: 03 Aug 2019 04:08


Tgt Ion:228 Resp: 965

Ion Ratio Lower Upper

228 100

226 39.3 25.6 38.4#

229 31.6 17.6 26.4#

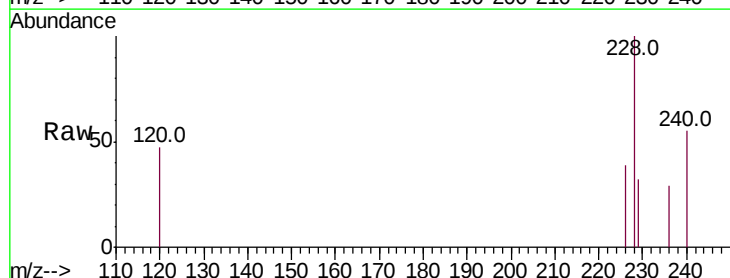

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

