
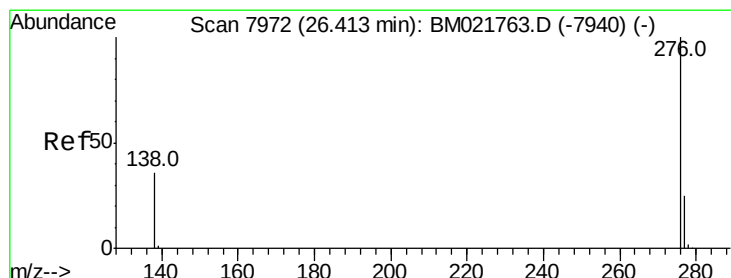
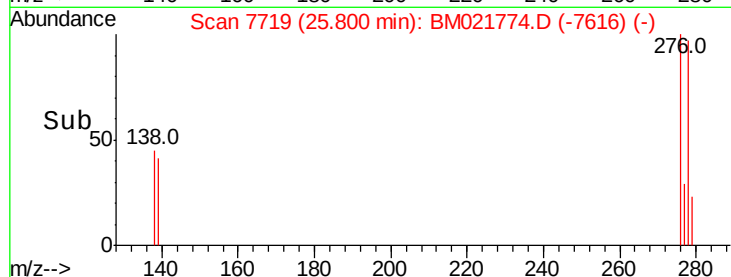
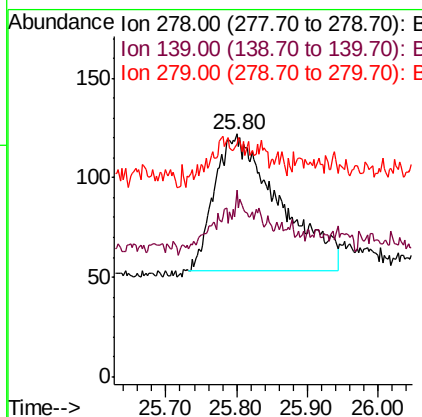


#25
Dibenzo(a,h)anthracene
Concen: 0.074 ng/ul
RT: 25.80 min Scan# 7719
Delta R.T. 0.05 min
Lab File: BM021774.D
Acq: 03 Aug 2019 04:08

Instrument :
BNA_M
ClientSampleId :

Tot Ion:278 Resp: 440
Ion Ratio Lower Upper
278 100
139 77.0 29.5 44.3#
279 95.9 31.1 46.7#

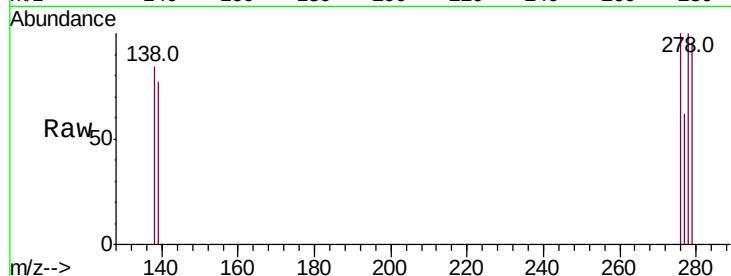

#26
Benzo(g,h,i)perylene
Concen: 0.080 ng/ul
RT: 26.44 min Scan# 7983
Delta R.T. 0.03 min
Lab File: BM021774.D
Acq: 03 Aug 2019 04:08

Tgt Ion:276 Resp: 588
Ion Ratio Lower Upper
276 100
138 67.1 36.2 54.2#
277 49.4 24.2 36.2#

