

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
 Data File : BM031444.D
 Acq On : 04 Aug 2021 13:01
 Operator : CG/JU
 Sample : M3122-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGEM7

Quant Time: Aug 04 14:26:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 12:17:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	1176	0.400	ng/ul	0.00
4) Naphthalene-d8	10.356	136	4505	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164	3183	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	6180	0.400	ng/ul	0.00
17) Chrysene-d12	21.169	240	5200	0.400	ng/ul	0.00
23) Perylene-d12	23.326	264	5668	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	5733	4.389	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.953	152	2404	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.005	212	6369	0.367	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.406	128	286	0.021	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
Data File : BM031444.D
Acq On : 04 Aug 2021 13:01
Operator : CG/JU
Sample : M3122-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGEM7


Quant Time: Aug 04 14:26:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 12:17:22 2021
Response via : Initial Calibration

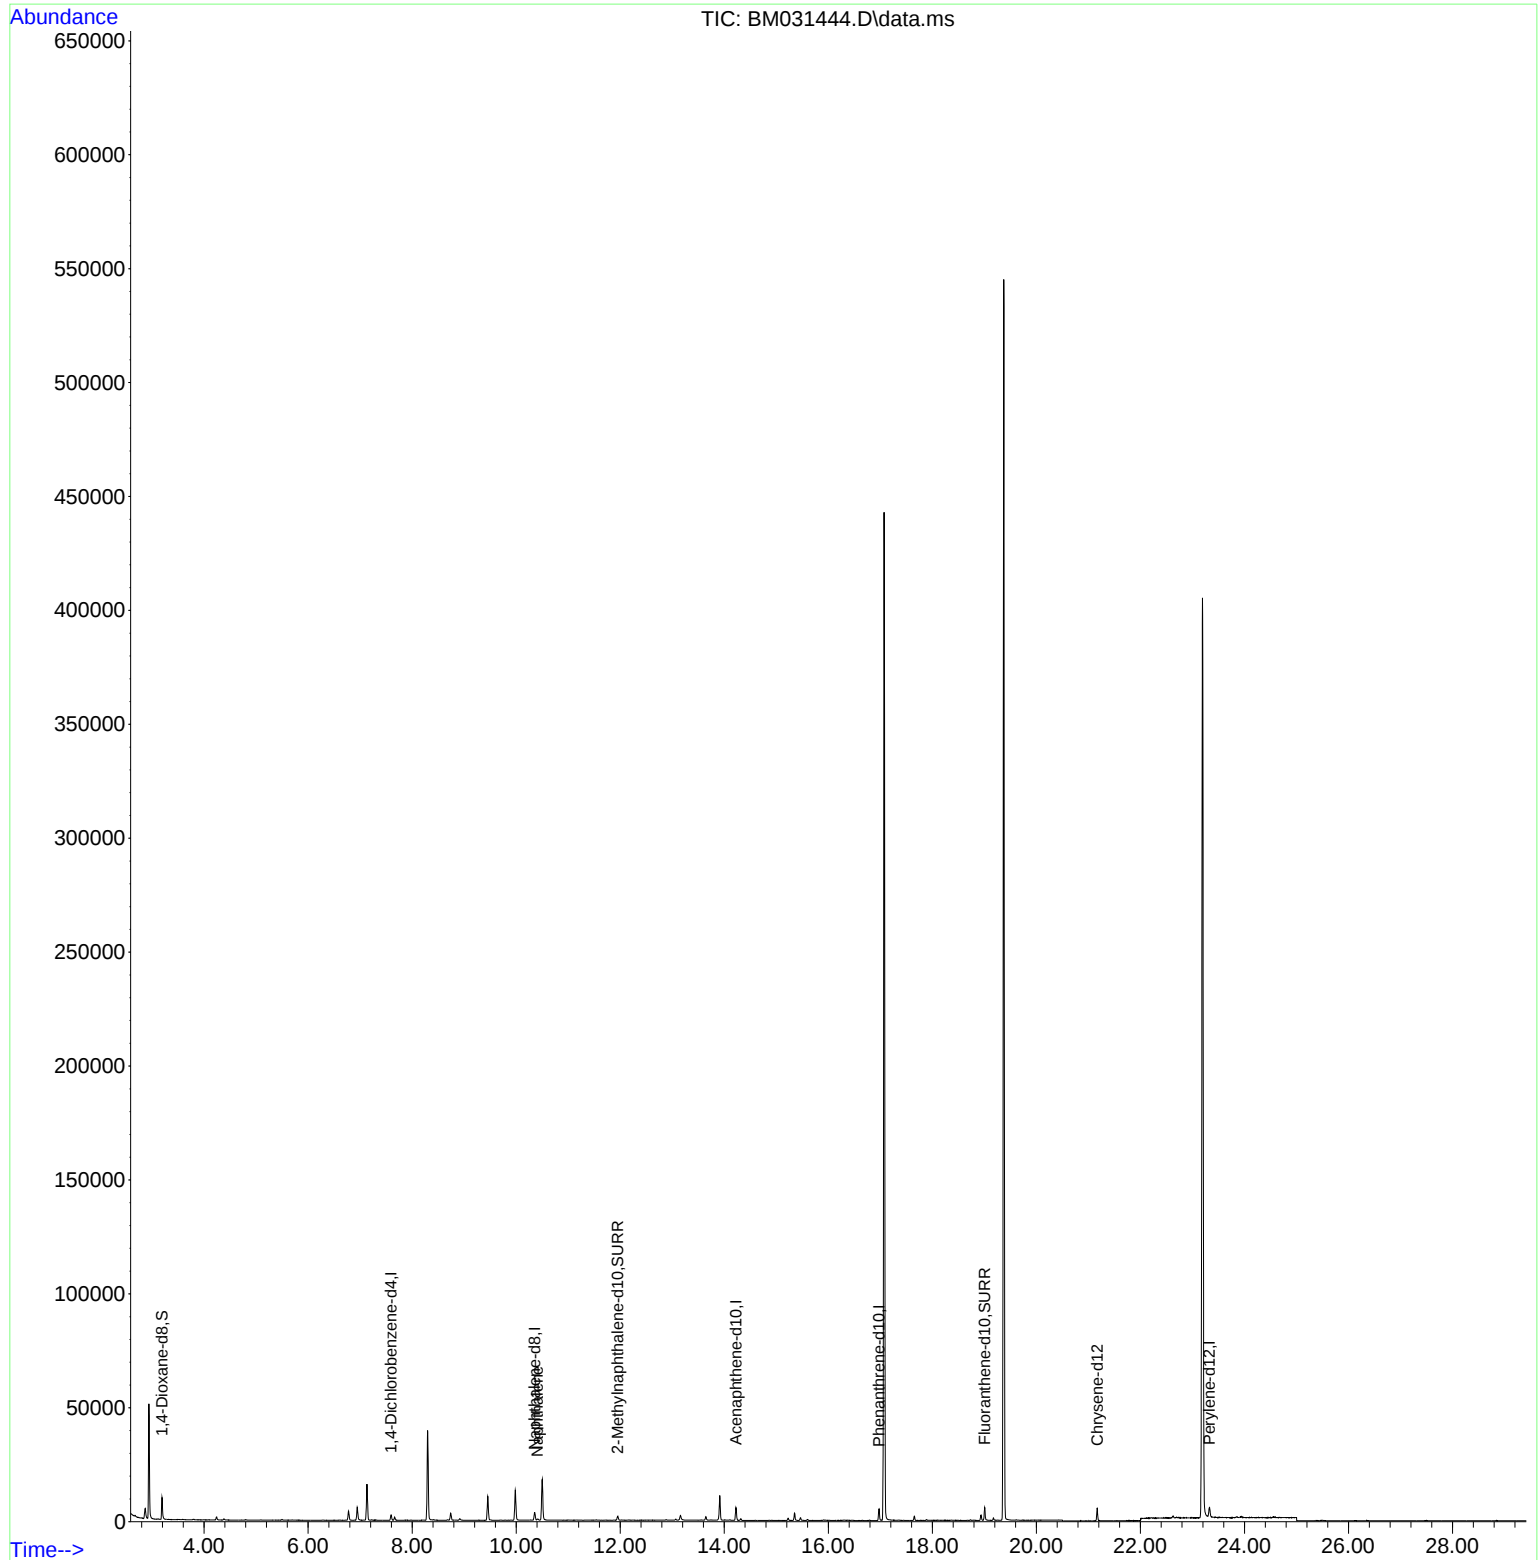

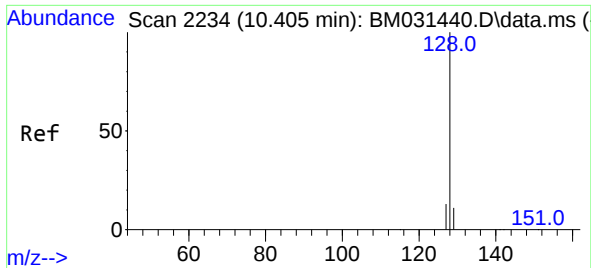

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.406 min Scan# 2234
Delta R.T. 0.001 min
Lab File: BM031444.D
Acq: 04 Aug 2021 13:01

Instrument :
BNA_M
ClientSampleId :
BGEM7

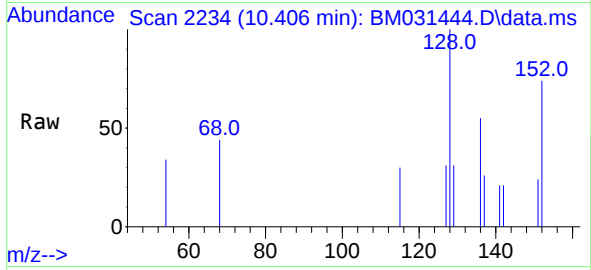

Tgt Ion:128 Resp: 286
Ion Ratio Lower Upper
128 100
129 30.8 10.0 15.0#
127 30.8 11.6 17.4#

