

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
 Data File : BM031445.D
 Acq On : 04 Aug 2021 13:38
 Operator : CG/JU
 Sample : M3124-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0061

Quant Time: Aug 04 14:27:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 12:17:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.594	152	1166	0.400	ng/ul	0.00
4) Naphthalene-d8	10.356	136	4516	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164	3074	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.975	188	5810	0.400	ng/ul	0.00
17) Chrysene-d12	21.169	240	4847	0.400	ng/ul	0.00
23) Perylene-d12	23.326	264	5127	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.189	96	5967	4.608	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.948	152	2906	0.382	ng/ul	0.00
18) Fluoranthene-d10	19.005	212	7304	0.452	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.401	128	440	0.033	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
Data File : BM031445.D
Acq On : 04 Aug 2021 13:38
Operator : CG/JU
Sample : M3124-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0061

Quant Time: Aug 04 14:27:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 12:17:22 2021
Response via : Initial Calibration

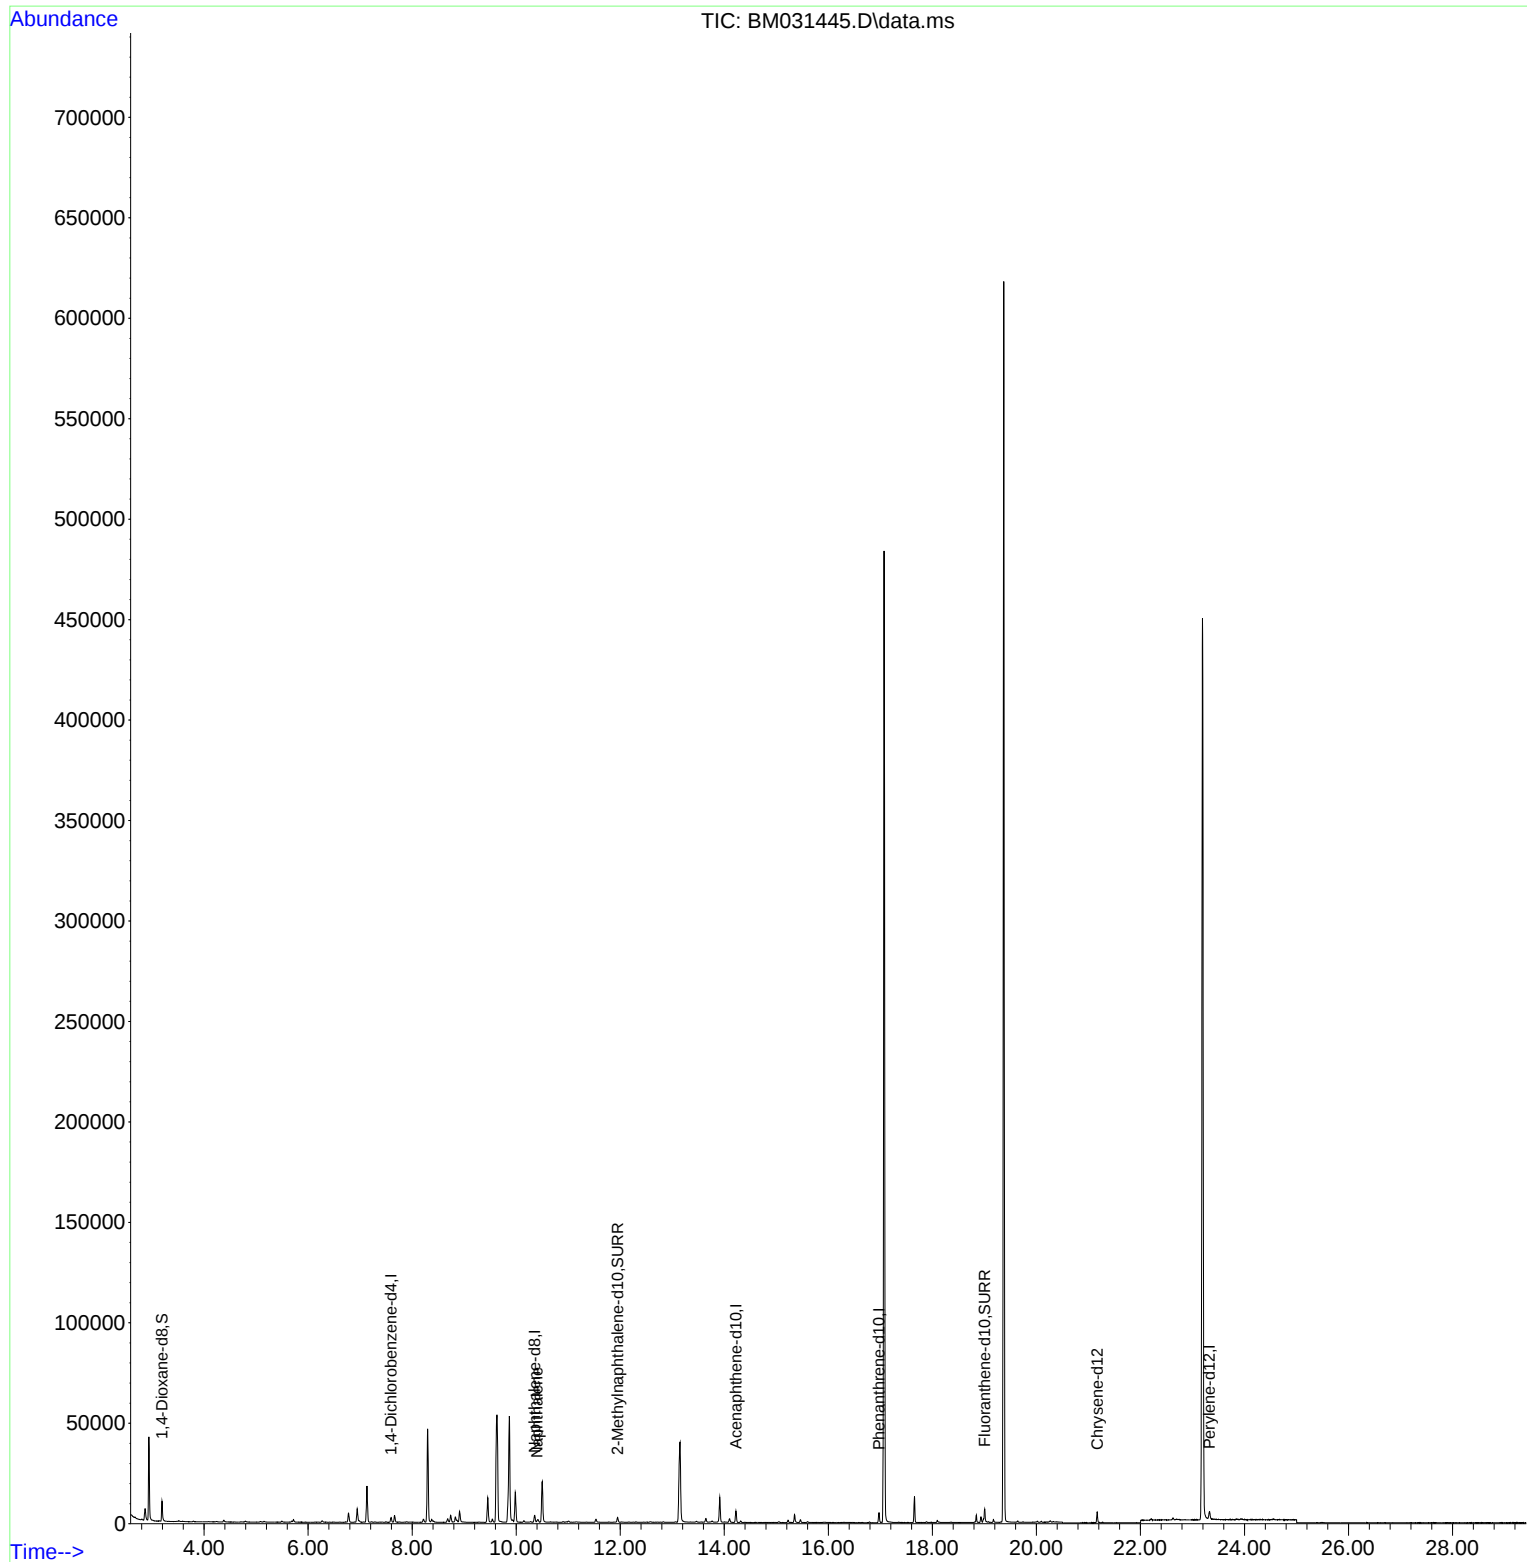

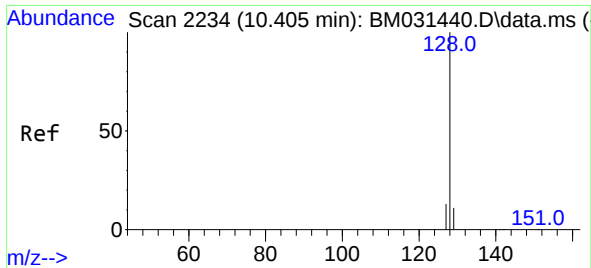

#5
Naphthalene
Concen: 0.033 ng/ul
RT: 10.401 min Scan# 2233
Delta R.T. -0.003 min
Lab File: BM031445.D
Acq: 04 Aug 2021 13:38

Instrument :
BNA_M
ClientSampleId :
C0061

Tgt Ion:128 Resp: 440
Ion Ratio Lower Upper
128 100
129 26.9 10.0 15.0#
127 28.2 11.6 17.4#

