

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
 Data File : BM031474.D
 Acq On : 05 Aug 2021 08:02
 Operator : CG/JU
 Sample : M3141-13
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BGER1

Quant Time: Aug 05 08:42:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 05 07:10:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.590	152	1502	0.400	ng/ul	0.00
4) Naphthalene-d8	10.352	136	5706	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.224	164	3531	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.971	188	6915	0.400	ng/ul	0.00
17) Chrysene-d12	21.164	240	5731	0.400	ng/ul	0.00
23) Perylene-d12	23.322	264	6176	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.189	96	5913	3.545	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.949	152	2050	0.213	ng/ul	0.00
18) Fluoranthene-d10	19.001	212	4318	0.226	ng/ul	0.00
Target Compounds						
						Qvalue
10) Acenaphthylene	13.946	152	2142	0.142	ng/ul	96
16) Anthracene	17.103	178	1169	0.057	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080221\
Data File : BM031474.D
Acq On : 05 Aug 2021 08:02
Operator : CG/JU
Sample : M3141-13
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BGER1


Quant Time: Aug 05 08:42:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM072821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 05 07:10:43 2021
Response via : Initial Calibration

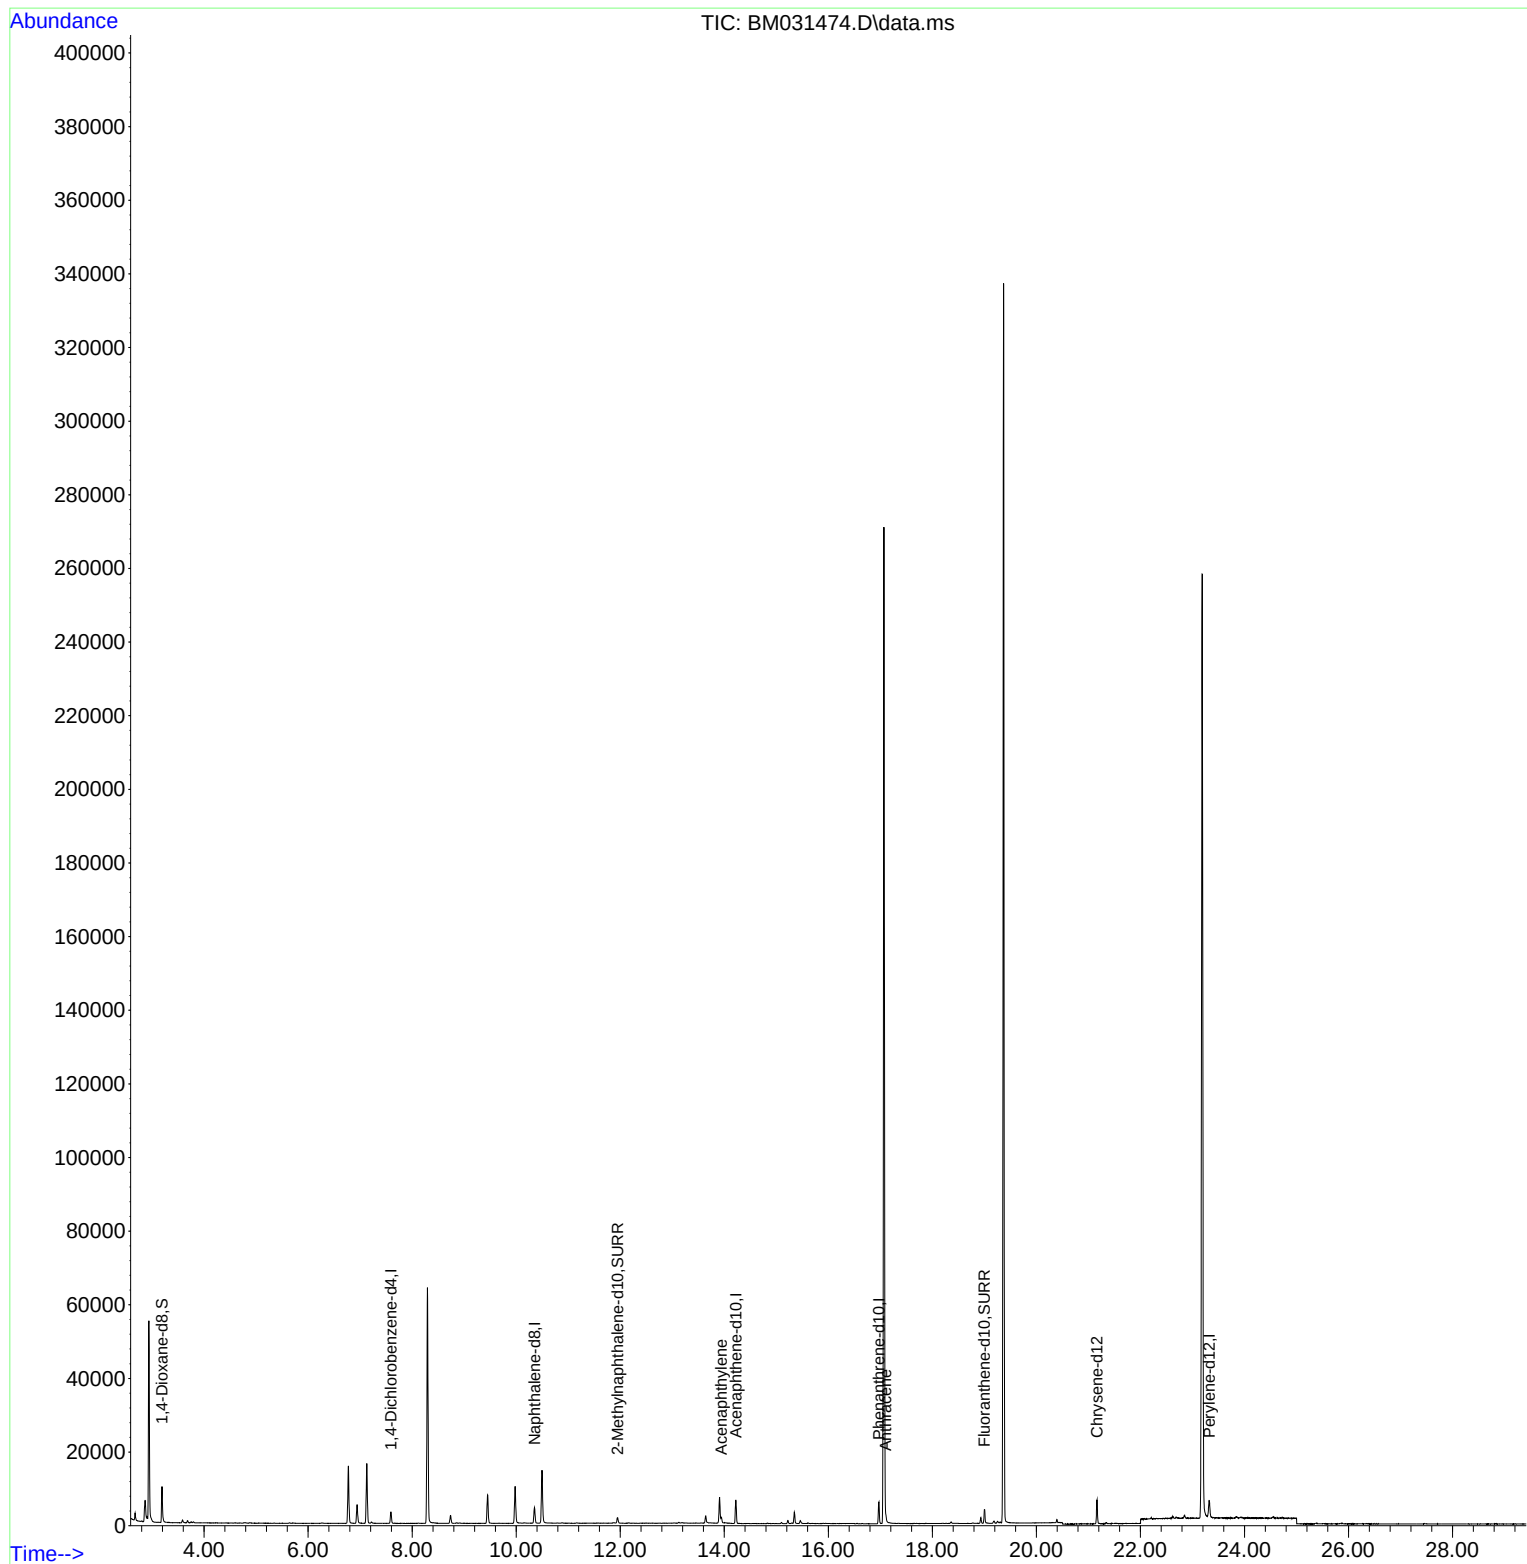



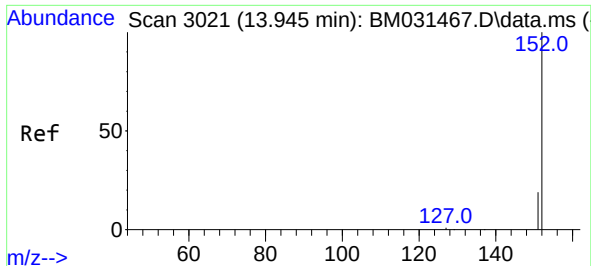


#10
Acenaphthylene
Concen: 0.142 ng/ul
RT: 13.946 min Scan# 3021
Delta R.T. -0.003 min
Lab File: BM031474.D
Acq: 05 Aug 2021 08:02

Instrument :
BNA_M
ClientSampled :
BGER1

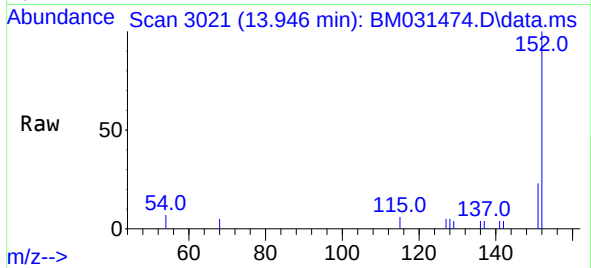

Tgt Ion:152 Resp: 2142
Ion Ratio Lower Upper
152 100
151 23.1 16.9 25.3
153 0.0 0.0 0.0

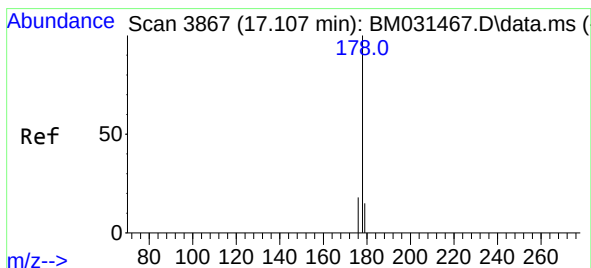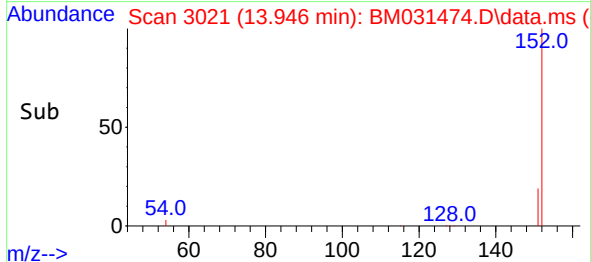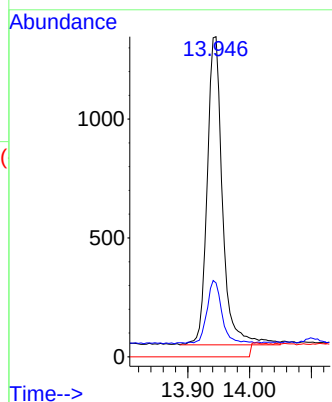

#16
Anthracene
Concen: 0.057 ng/ul
RT: 17.103 min Scan# 3866
Delta R.T. -0.006 min
Lab File: BM031474.D
Acq: 05 Aug 2021 08:02

Tgt Ion:178 Resp: 1169
Ion Ratio Lower Upper
178 100
179 24.2 13.0 19.6#
176 26.9 15.6 23.4#

