
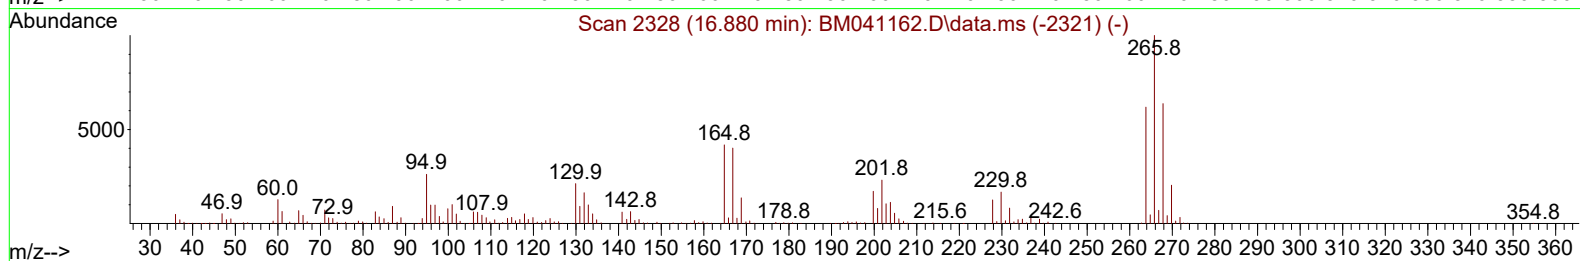
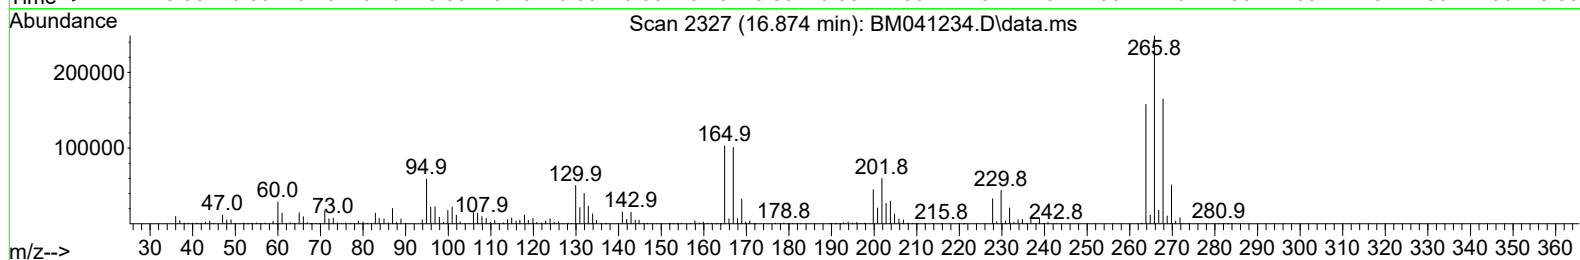


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041234.D
Acq On : 02 Aug 2023 08:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 08:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

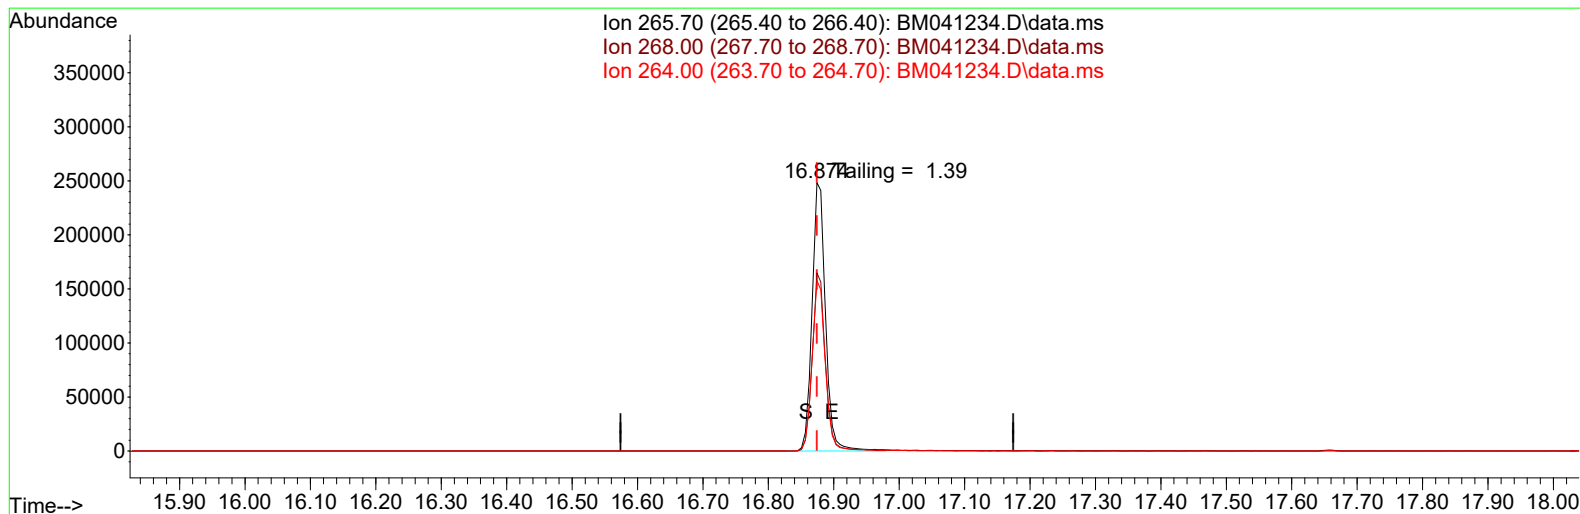

TIC: BM041234.D\data.ms

(70) Pentachlorophenol (C)




16.874min (0.000) 0.00 ng

response 357874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	66.37
264.00	61.80	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041234.D
Acq On : 02 Aug 2023 08:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 08:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

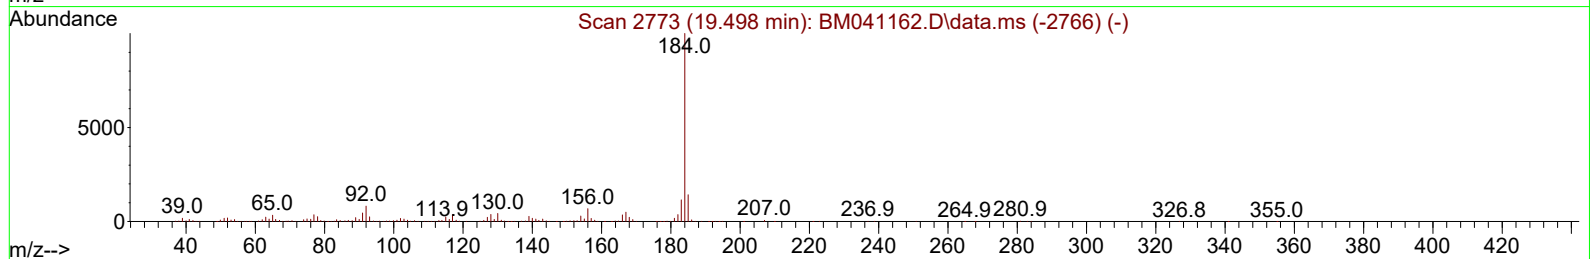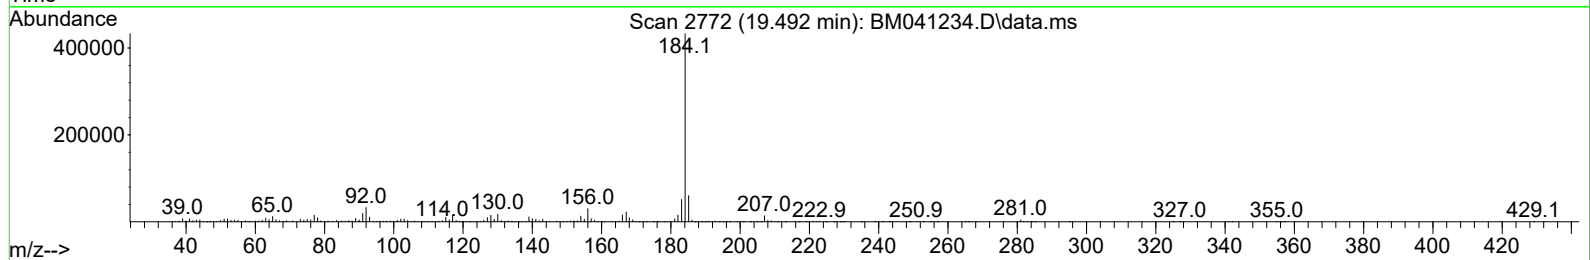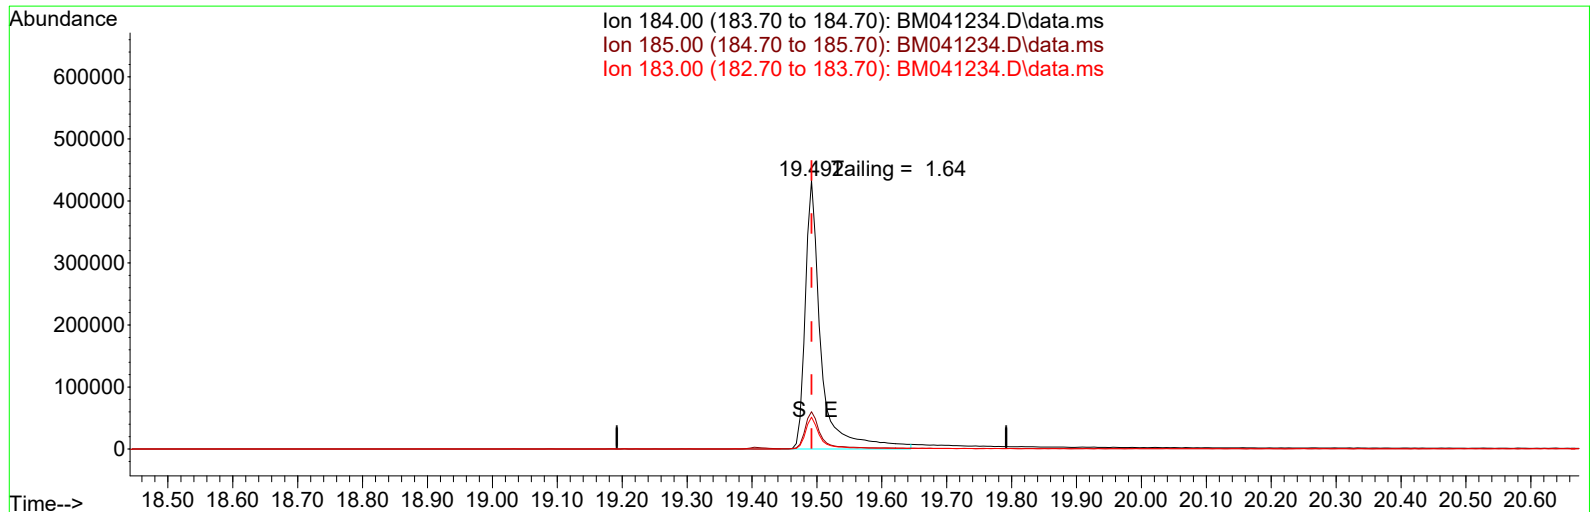

TIC: BM041234.D\data.ms

(77) Benzidine**19.492min (0.000) 108264.93 ng****response 745198**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.88
183.00	11.50	11.88
0.00	0.00	0.00