

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
 Data File : BM041248.D
 Acq On : 02 Aug 2023 17:07
 Operator : MA/JU
 Sample : 03810-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 WC-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM041248.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	365	371	388	rBV	2668842	3911188	43.05%	6.884%
2	6.987	638	646	658	rBV	2703916	4333516	47.70%	7.627%
3	7.798	774	784	792	rBV	753253	1185650	13.05%	2.087%
4	8.975	975	984	999	rBV	1762155	2813729	30.97%	4.952%
5	10.604	1251	1261	1273	rBV	1057413	1744123	19.20%	3.070%
6	13.080	1675	1682	1695	rBV	4862443	6899714	75.95%	12.144%
7	14.463	1911	1917	1924	rBV	1651353	2390650	26.32%	4.208%
8	15.968	2166	2173	2192	rVB	4160385	5775829	63.58%	10.166%
9	17.227	2378	2387	2391	rBV	1989103	2848104	31.35%	5.013%
10	17.262	2391	2393	2397	rVB	162844	208682	2.30%	0.367%
11	17.351	2404	2408	2413	rVB2	58965	101838	1.12%	0.179%
12	18.127	2532	2540	2550	rBV2	1676571	2614213	28.78%	4.601%
13	18.239	2555	2559	2564	rVV2	69425	129857	1.43%	0.229%
14	18.292	2564	2568	2573	rVV2	163244	322751	3.55%	0.568%
15	18.339	2573	2576	2583	rVB	95562	132210	1.46%	0.233%
16	19.027	2688	2693	2698	rBV2	163433	297773	3.28%	0.524%
17	19.292	2730	2738	2745	rBV	683040	1146901	12.62%	2.019%
18	19.409	2753	2758	2766	rBV	771822	1092380	12.02%	1.923%
19	19.474	2767	2769	2776	rVV3	106254	163365	1.80%	0.288%
20	19.545	2777	2781	2791	rVB3	196413	289009	3.18%	0.509%
21	19.627	2791	2795	2796	rBV	123906	141071	1.55%	0.248%
22	19.656	2796	2800	2808	rVB	694811	982741	10.82%	1.730%
23	19.862	2829	2835	2840	rBV	7678437	9084637	100.00%	15.990%
24	19.986	2852	2856	2865	rVB2	81111	202263	2.23%	0.356%
25	20.315	2909	2912	2914	rBV	120065	148141	1.63%	0.261%
26	20.451	2933	2935	2939	rVB	121424	130106	1.43%	0.229%
27	20.498	2940	2943	2947	rVB	153689	180276	1.98%	0.317%
28	20.662	2968	2971	2975	rVB2	124551	139056	1.53%	0.245%
29	21.133	3047	3051	3059	rVB2	880857	1264095	13.91%	2.225%
30	21.333	3083	3085	3088	rVB	194432	170570	1.88%	0.300%
31	21.427	3095	3101	3105	rBV2	1919217	2802231	30.85%	4.932%
32	21.462	3105	3107	3113	rVB	339299	394660	4.34%	0.695%
33	22.021	3199	3202	3205	rVB	385119	414763	4.57%	0.730%
34	22.050	3205	3207	3214	rVB	285525	385229	4.24%	0.678%
35	23.803	3499	3505	3511	rVB	1081335	1974379	21.73%	3.475%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041248.D
Acq On : 02 Aug 2023 17:07
Operator : MA/JU
Sample : 03810-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION




Sum of corrected areas: 56815700

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041248.D
Acq On : 02 Aug 2023 17:07
Operator : MA/JU
Sample : 03810-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

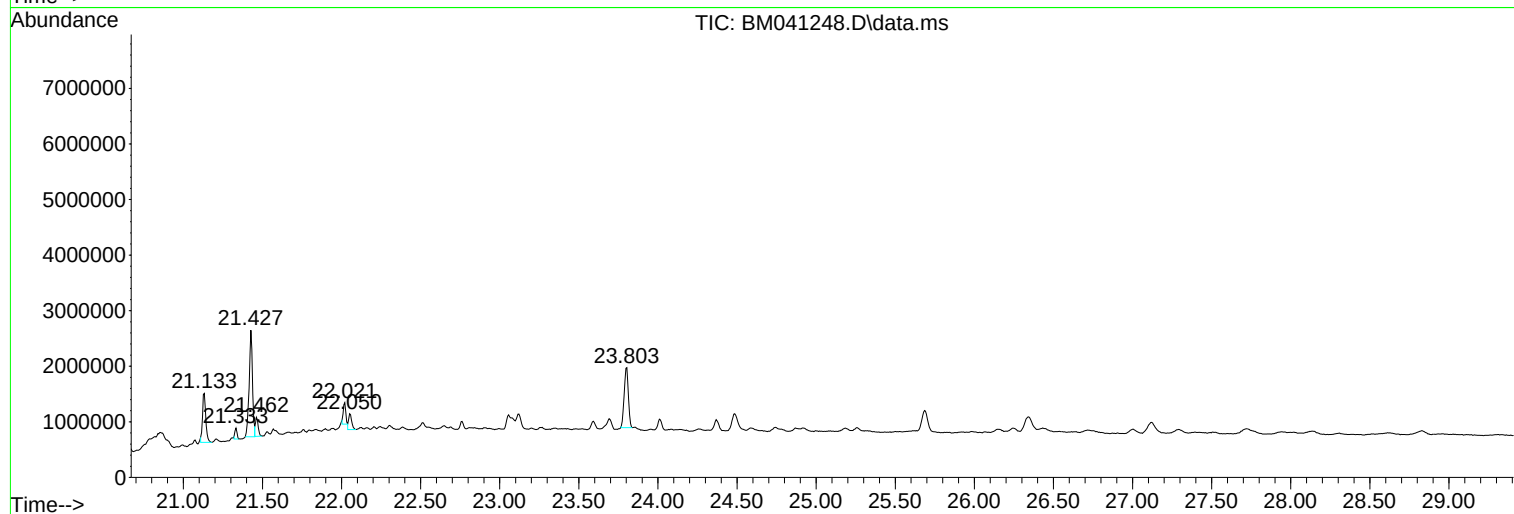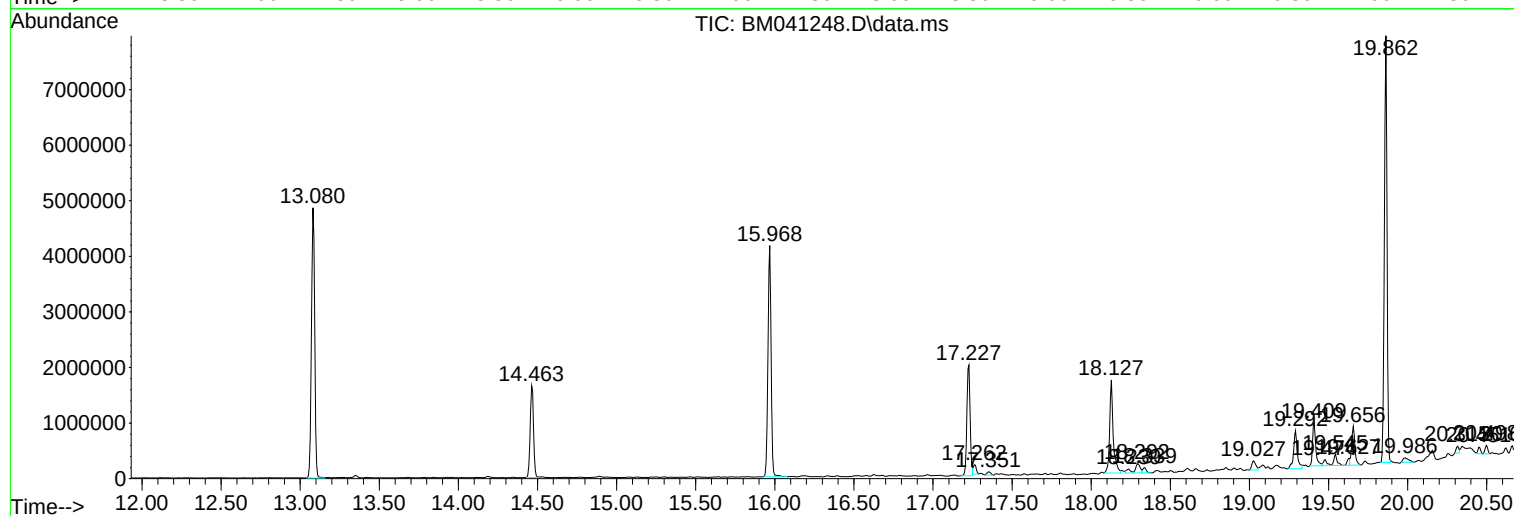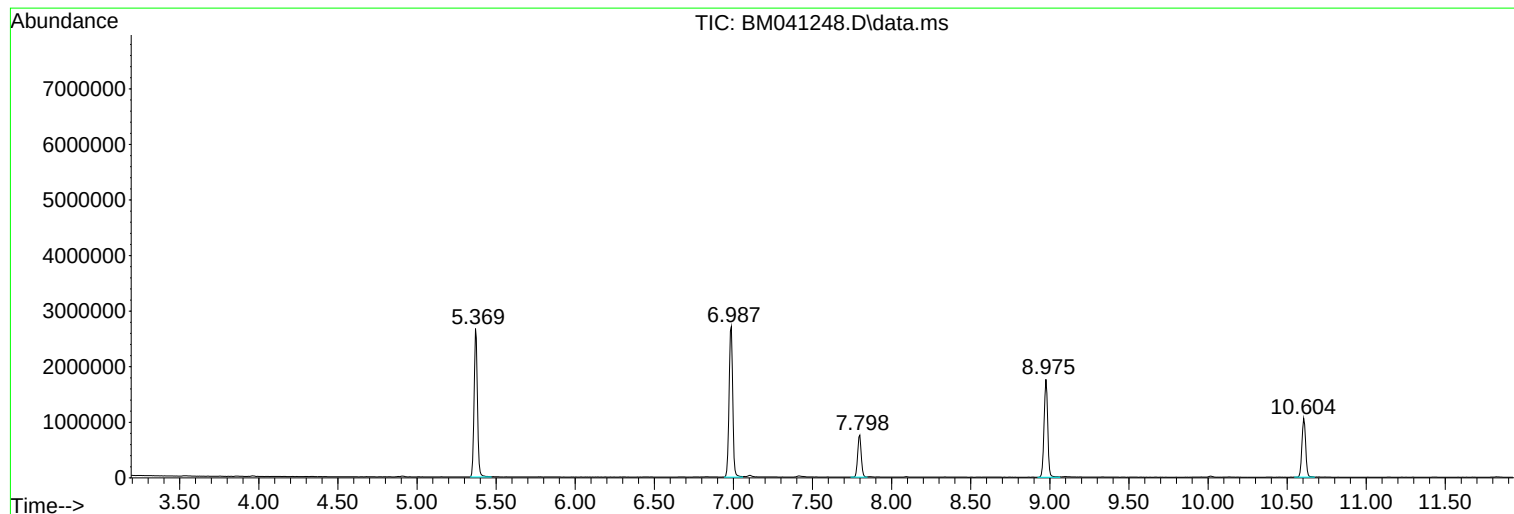

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041248.D
Acq On : 02 Aug 2023 17:07
Operator : MA/JU
Sample : 03810-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041248.D
Acq On : 02 Aug 2023 17:07
Operator : MA/JU
Sample : 03810-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
WC-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------