


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041234.D
Acq On : 02 Aug 2023 08:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 02 19:20:51 2023

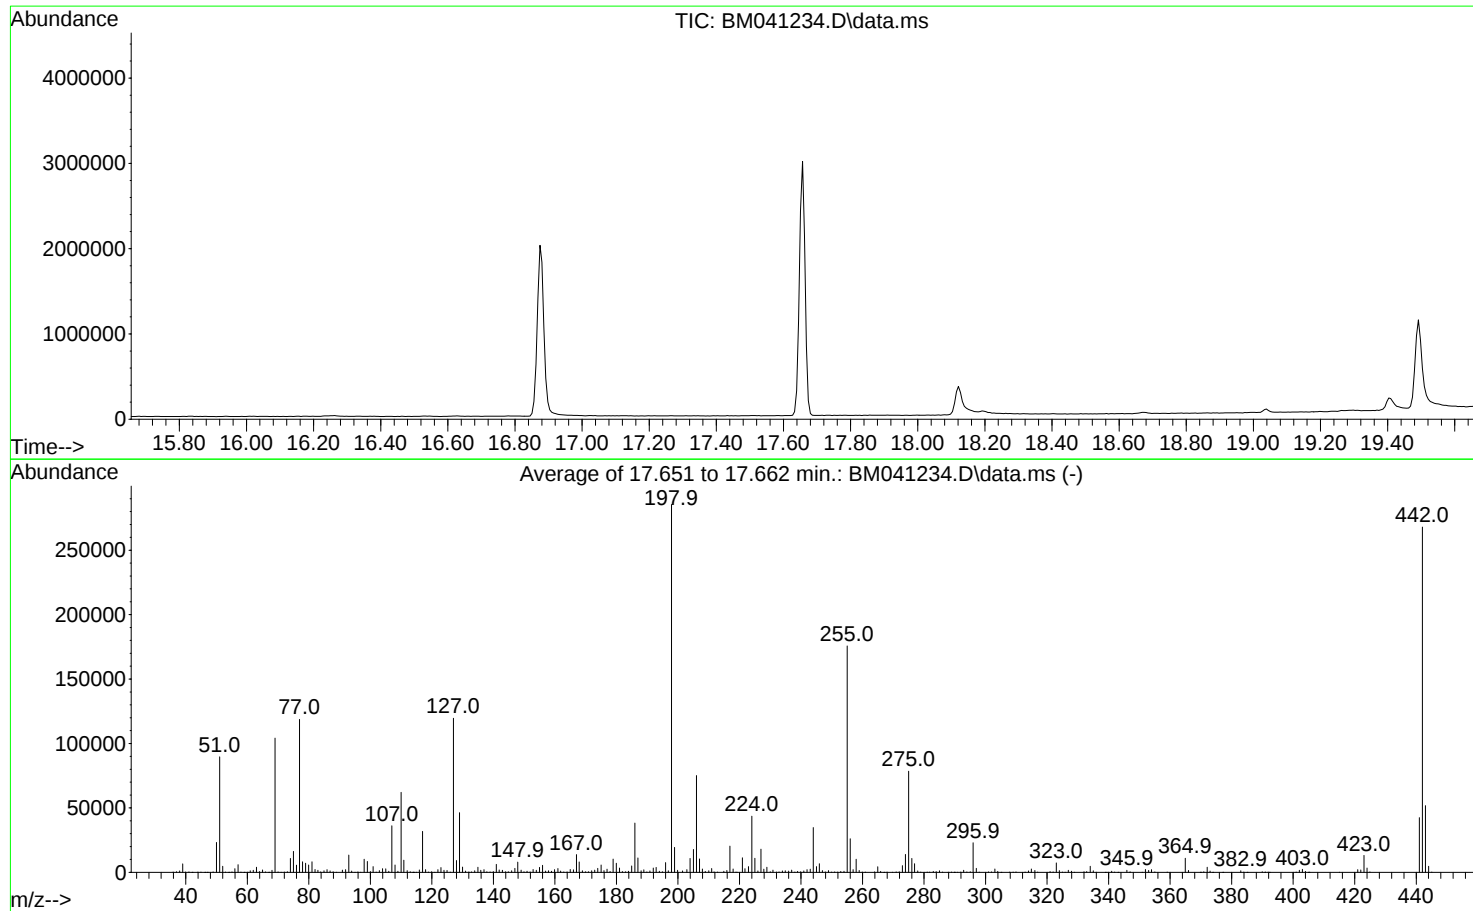

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	89715	PASS
68	69	0.00	2	1.5	1587	PASS
69	198	0.00	100	36.5	104236	PASS
70	69	0.00	2	0.4	417	PASS
127	198	10	80	41.9	119624	PASS
197	198	0.00	2	0.4	1236	PASS
198	198	100	100	100.0	285483	PASS
199	198	5	9	6.8	19424	PASS
275	198	10	60	27.5	78485	PASS
365	198	1	100	3.8	10966	PASS
441	198	0.01	100	14.9	42437	PASS
442	442	50	100	100.0	267947	PASS
443	442	15	24	19.4	51848	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_M	<u>BM041234.D</u>
Compound Name	Response	Retention Time
DDT	963042	20.715
DDD	23777	20.28
DDE	1186	19.762
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24963	988005	2.53

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
Data File : BM041234.D
Acq On : 02 Aug 2023 08:25
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Aug 02 08:57:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 31 16:29:28 2023
Response via : Initial Calibration

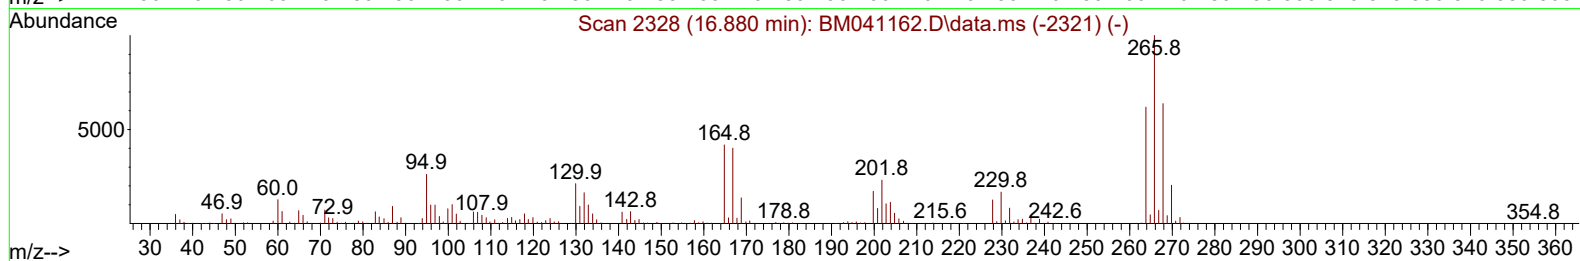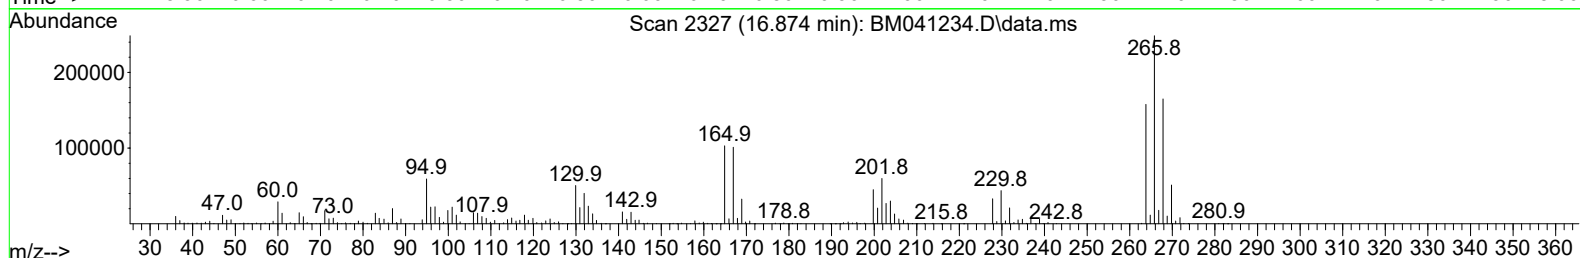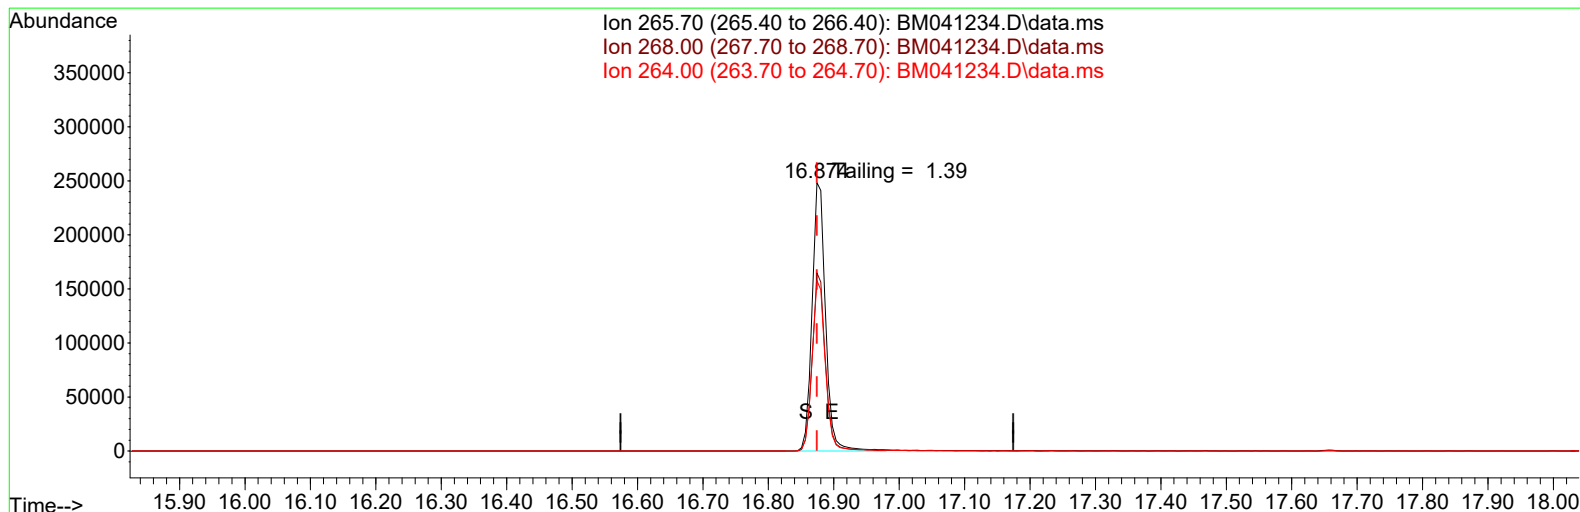

TIC: BM041234.D\data.ms

(70) Pentachlorophenol (C)

16.874min (0.000) 0.00 ng




response 357874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	66.37
264.00	61.80	63.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM080223\
 Data File : BM041234.D
 Acq On : 02 Aug 2023 08:25
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 08:57:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 31 16:29:28 2023
 Response via : Initial Calibration

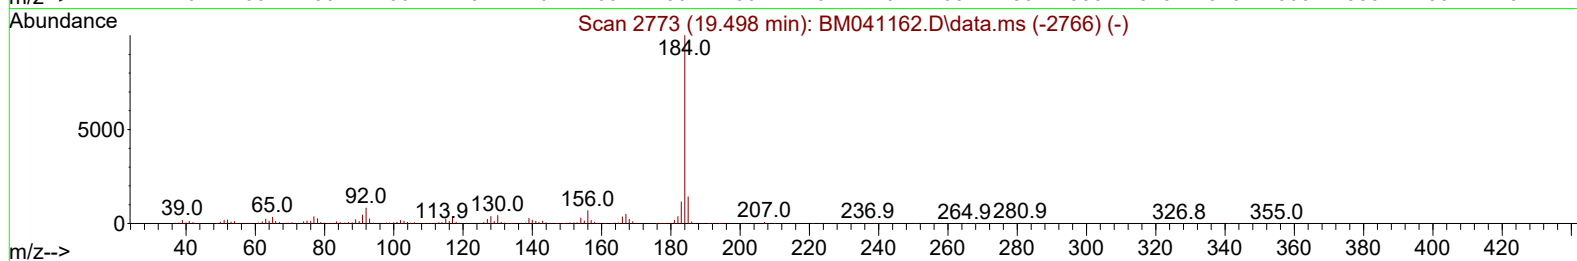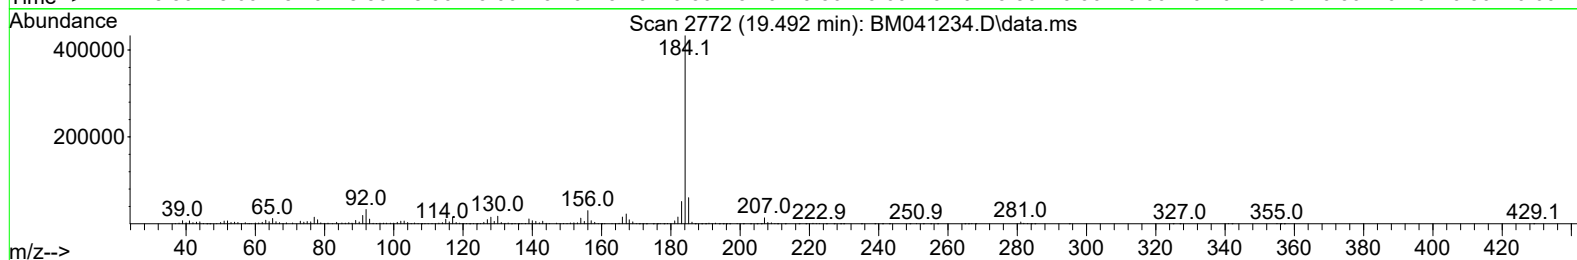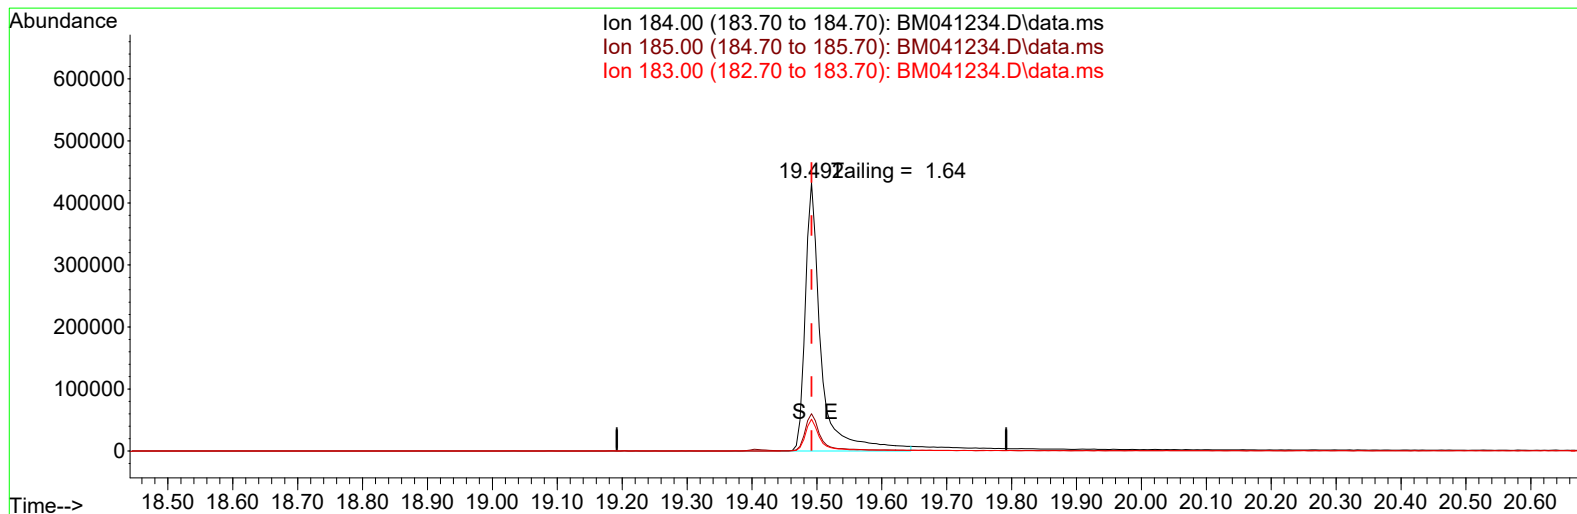

TIC: BM041234.D\data.ms

(77) Benzidine**19.492min (0.000) 108264.93 ng****response 745198**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.88
183.00	11.50	11.88
0.00	0.00	0.00