
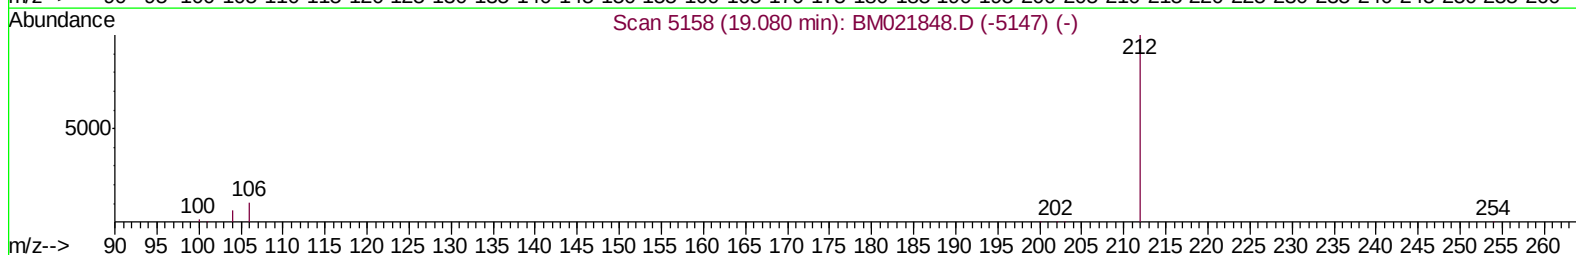
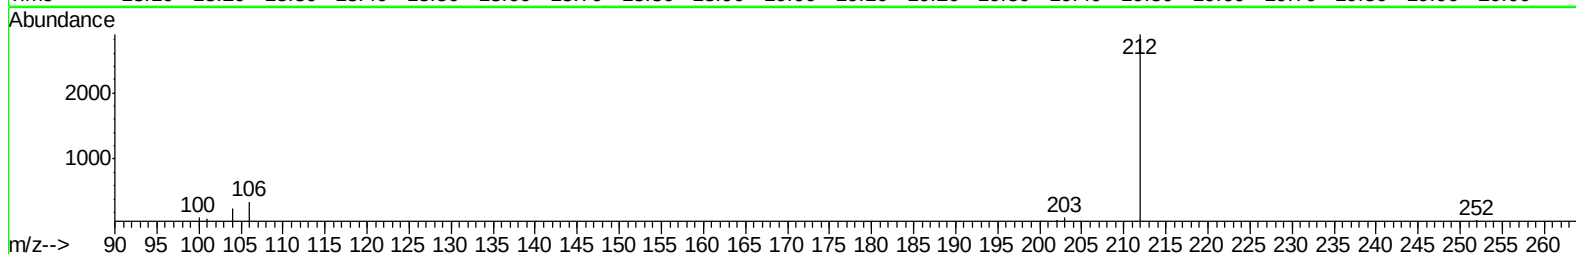


Data File : BM021849.D
Acq On : 05 Aug 2019 19:17
Operator : HP/JU
Sample : K3823-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 06 01:39:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

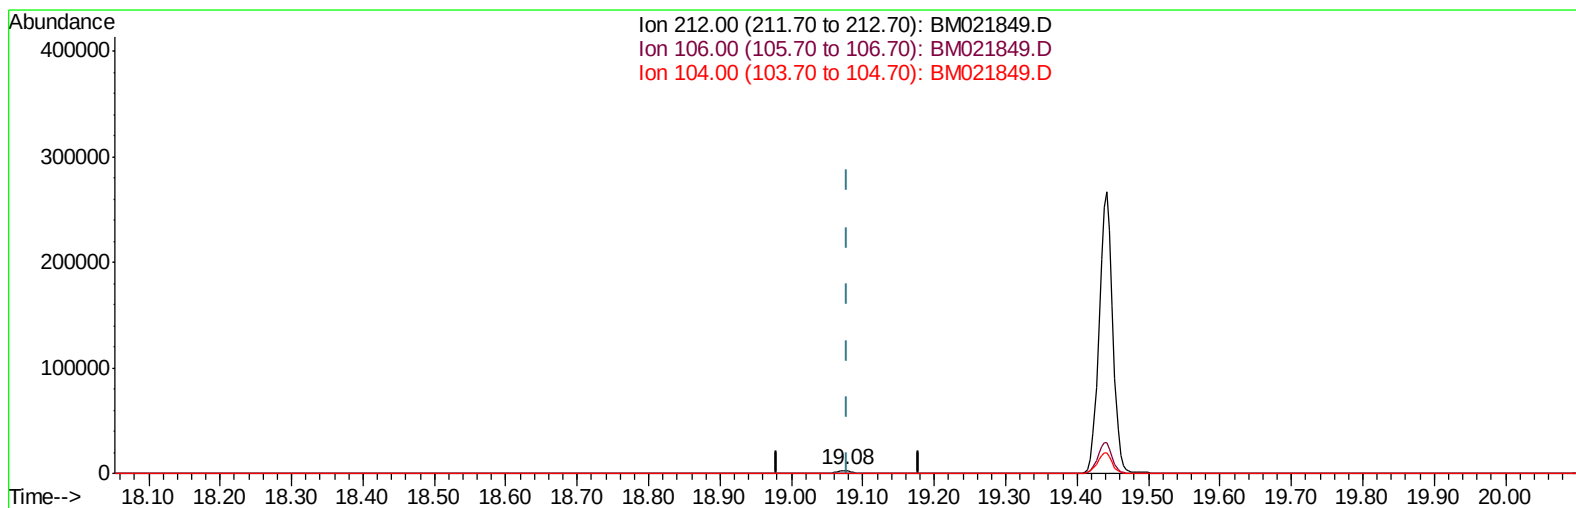

TIC: BM021849.D

(14) Fluoranthene-d10 (SURR)

19.076min (-0.004) 0.24ng/ul m

response 3911

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.00#
104.00	6.00	0.00#
0.00	0.00	0.00