
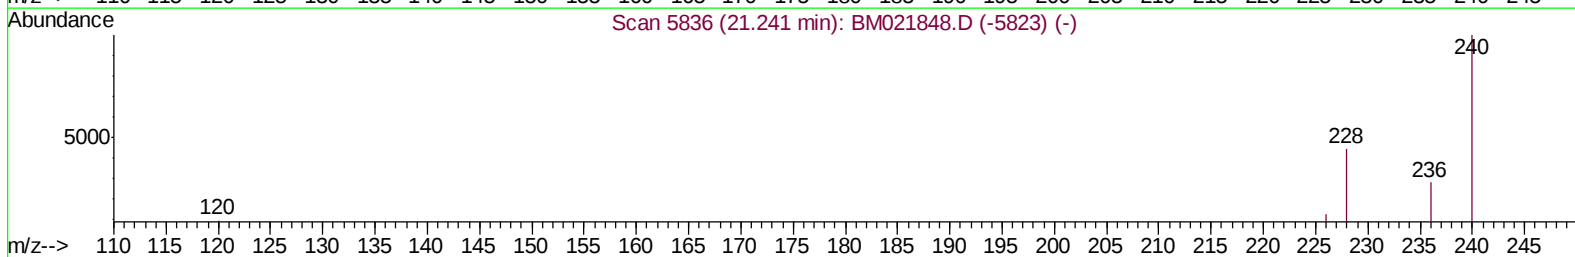
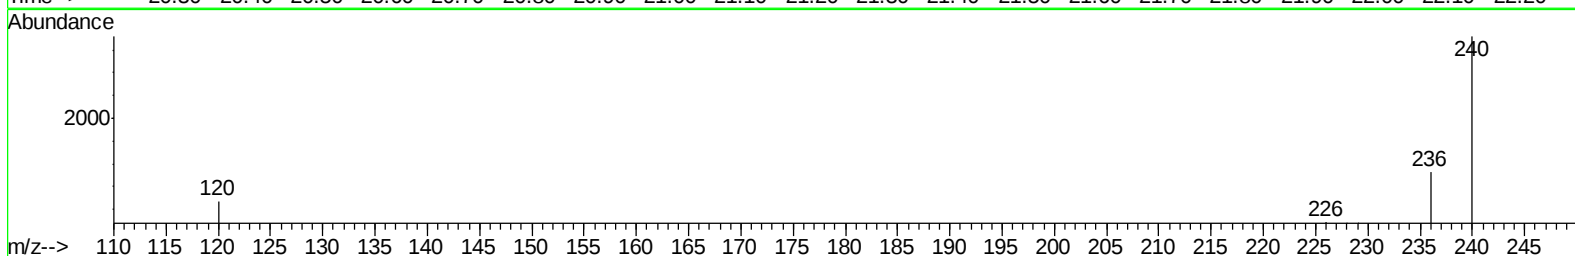


Data File : BM021849.D
Acq On : 05 Aug 2019 19:17
Operator : HP/JU
Sample : K3823-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Quant Time: Aug 06 01:39:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

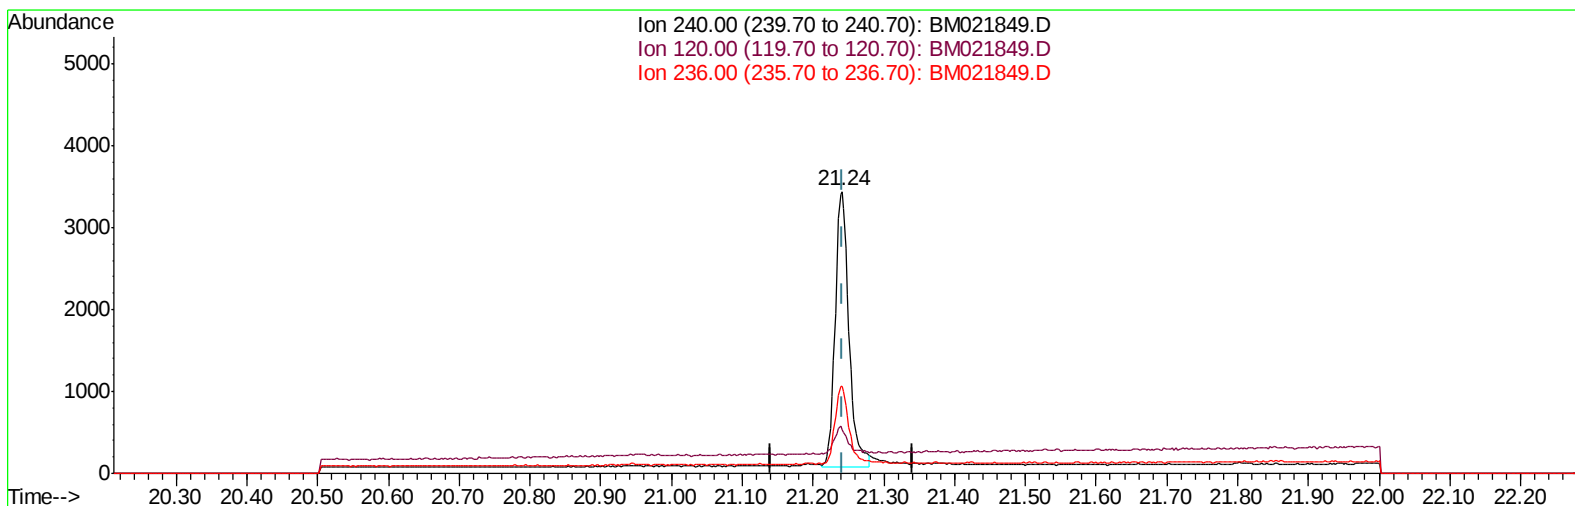

TIC: BM021849.D

(16) Chrysene-d12 (I)

21.241min (-0.000) 0.40ng/ul m

response 4565

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	15.65
236.00	32.30	30.81
0.00	0.00	0.00