
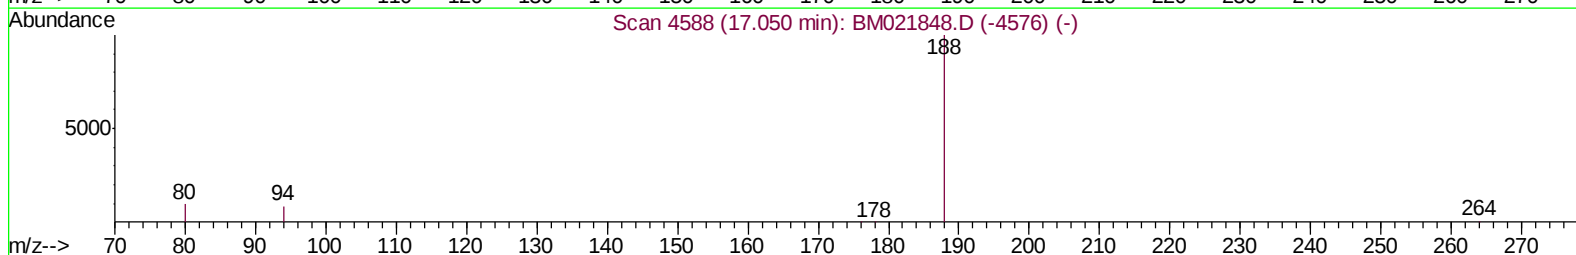
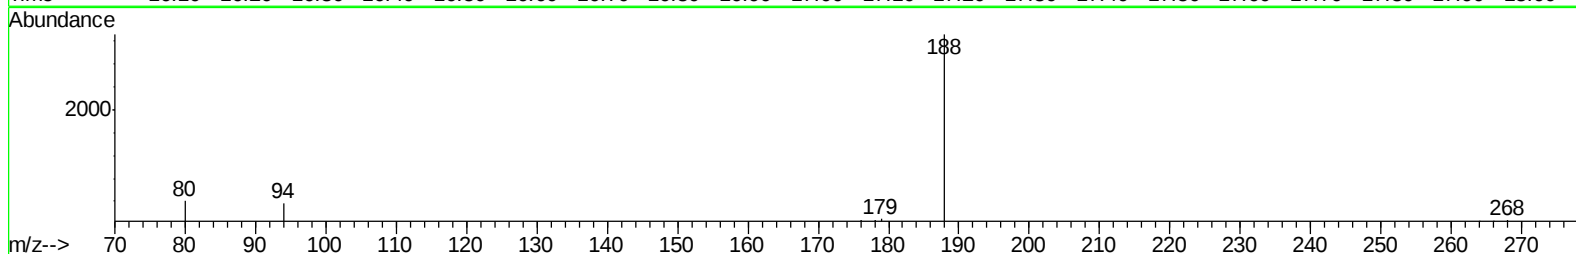


Data File : BM021850.D  
Acq On : 05 Aug 2019 19:54  
Operator : HP/JU  
Sample : K3823-14RE  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 06 01:32:08 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 06 01:29:26 2019  
Response via : Initial Calibration

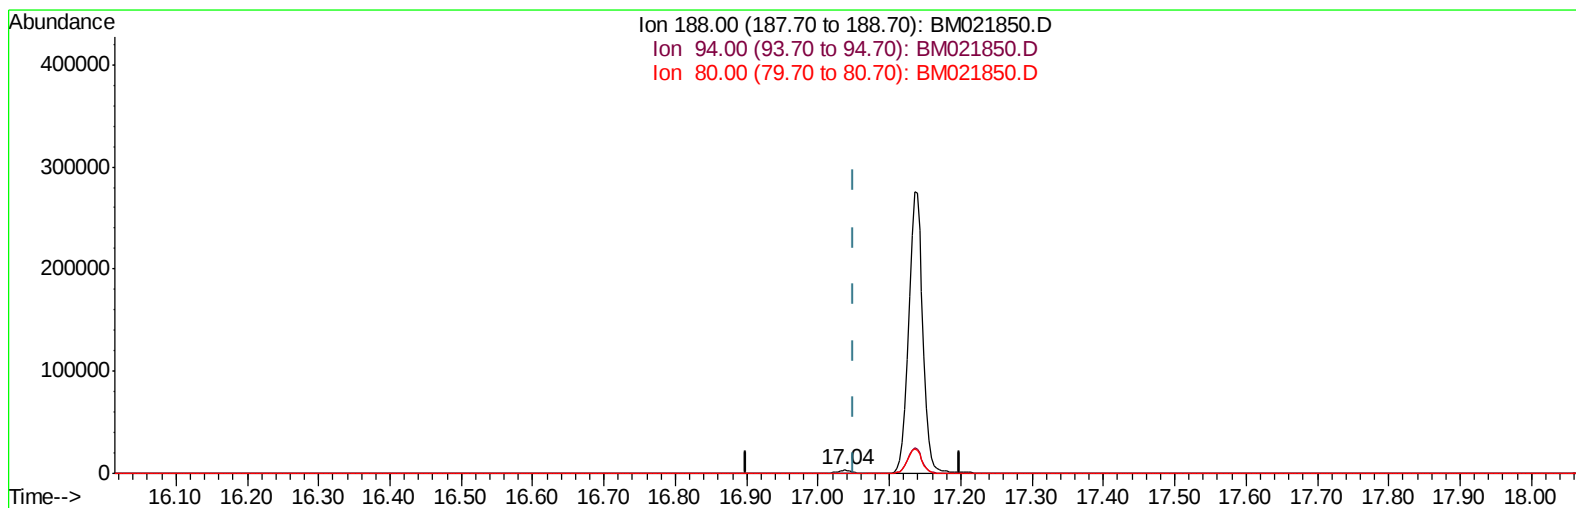

TIC: BM021850.D

(10) Phenanthrene-d10 (I)

17.038min (-0.012) 0.40ng/ul m

response 4730

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 188.00 | 100   | 100   |
| 94.00  | 10.40 | 10.92 |
| 80.00  | 11.40 | 12.00 |
| 0.00   | 0.00  | 0.00  |