
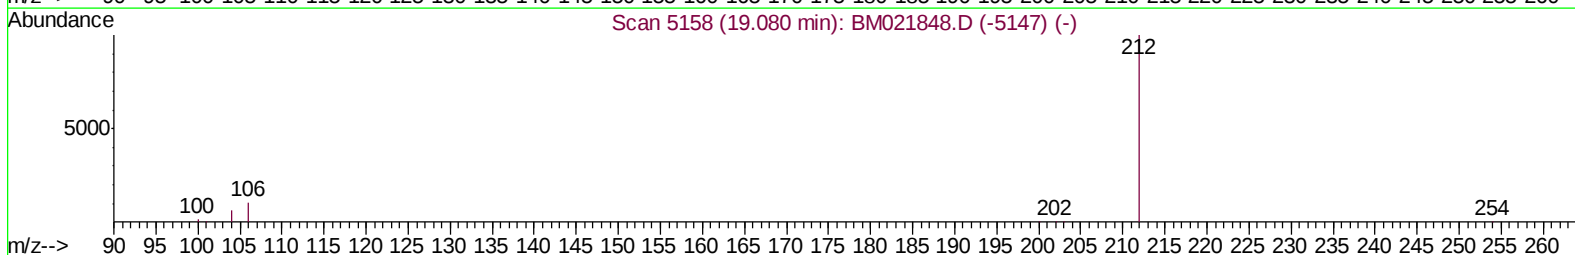
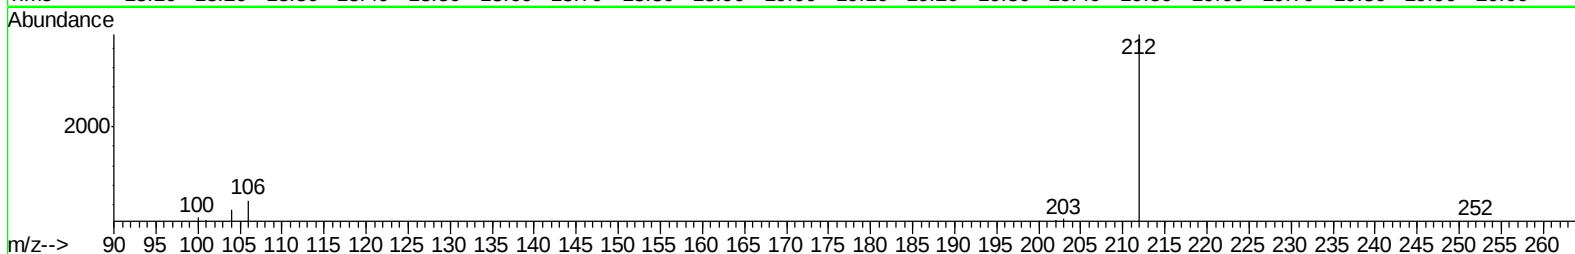


Data File : BM021850.D  
Acq On : 05 Aug 2019 19:54  
Operator : HP/JU  
Sample : K3823-14RE  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 06 01:42:25 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 06 01:29:26 2019  
Response via : Initial Calibration

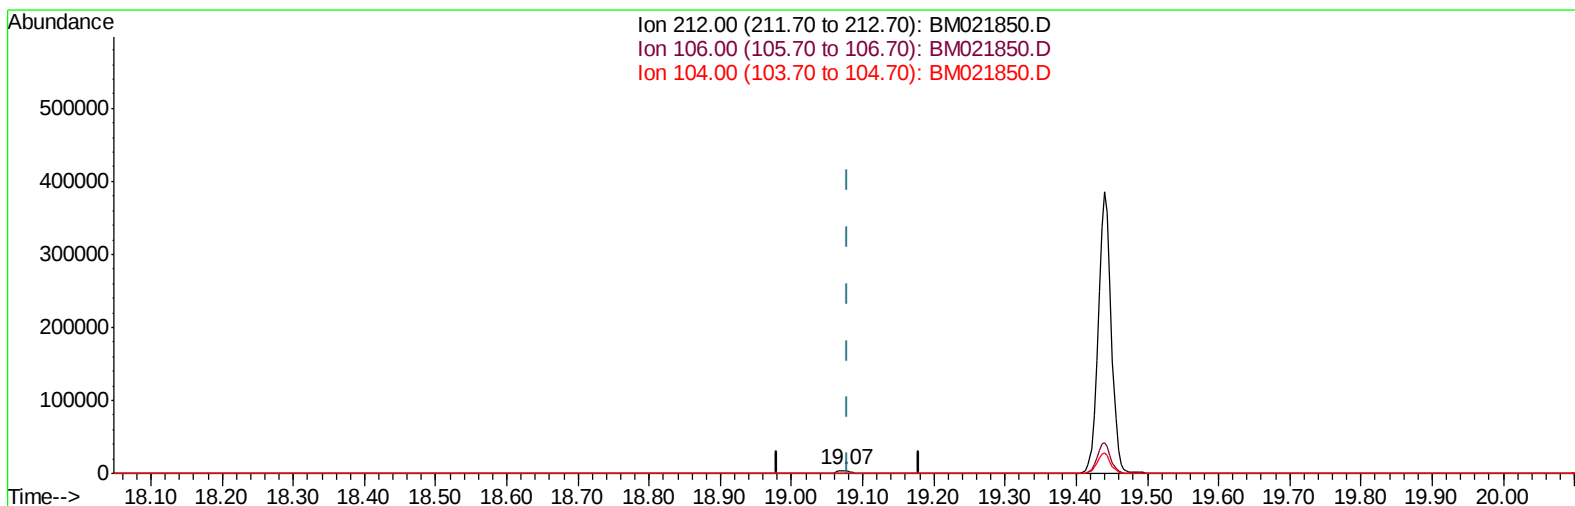

TIC: BM021850.D

(14) Fluoranthene-d10 (SURR)

19.074min (-0.006) 0.34ng/ul m

response 5380

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 212.00 | 100  | 100   |
| 106.00 | 9.90 | 0.00# |
| 104.00 | 6.00 | 0.00# |
| 0.00   | 0.00 | 0.00  |