
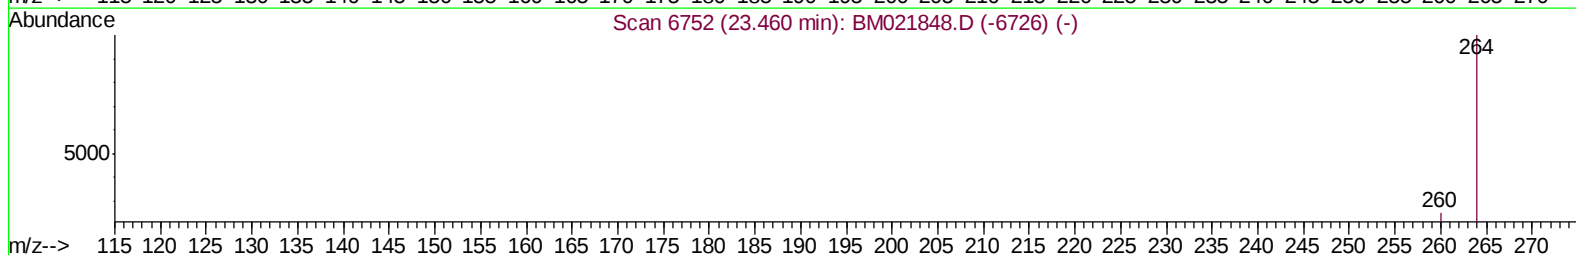
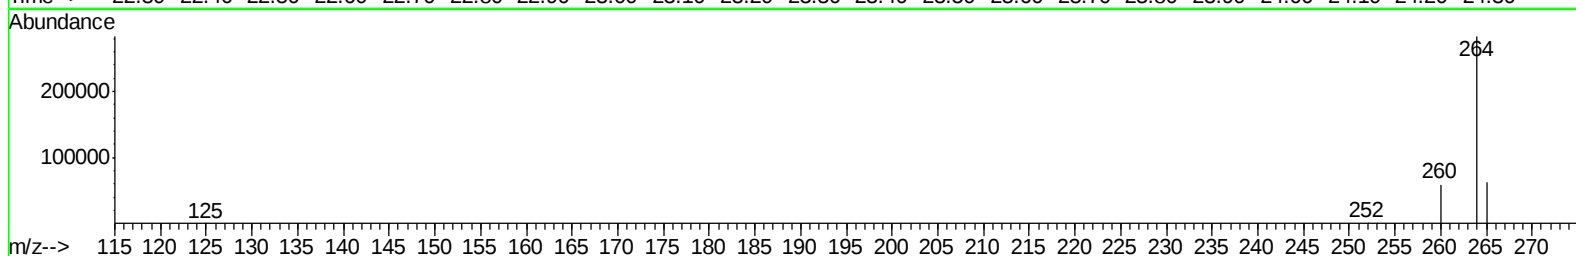


Data File : BM021850.D  
Acq On : 05 Aug 2019 19:54  
Operator : HP/JU  
Sample : K3823-14RE  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 06 01:43:08 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 06 01:29:26 2019  
Response via : Initial Calibration

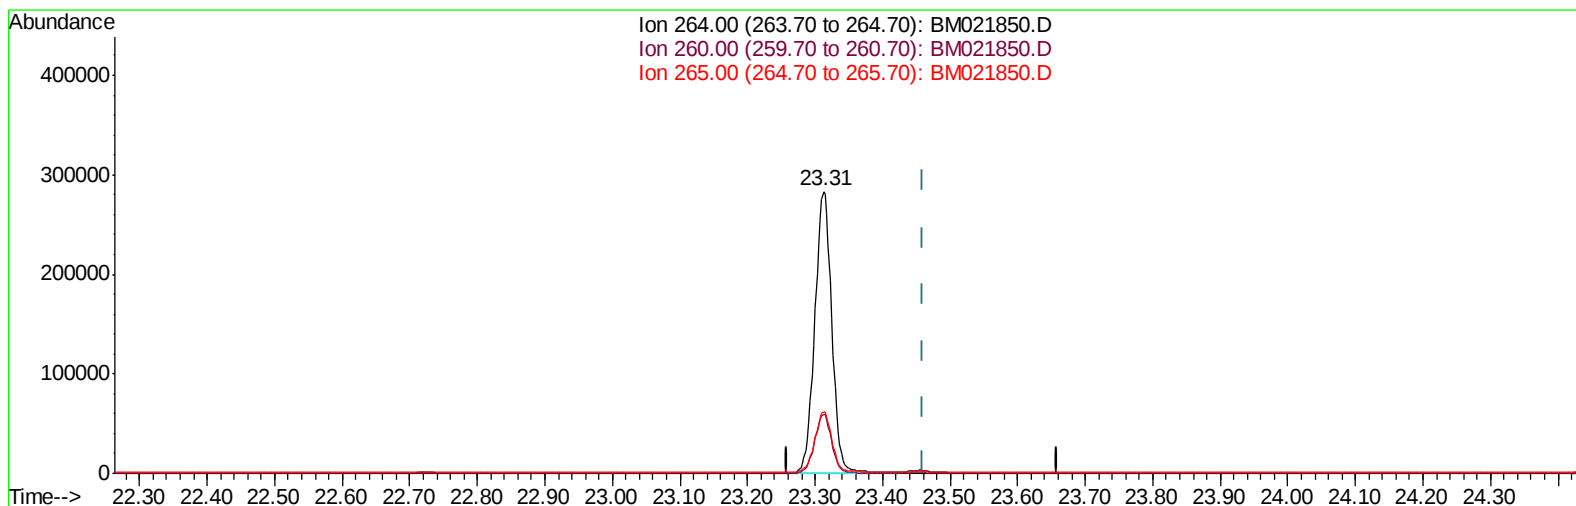

TIC: BM021850.D

(20) Perylene-d12 (I)  
23.312min (-0.147) 0.40ng/ul  
response 497516

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 27.50  | 21.07# |
| 265.00 | 117.00 | 21.92# |
| 0.00   | 0.00   | 0.00   |