
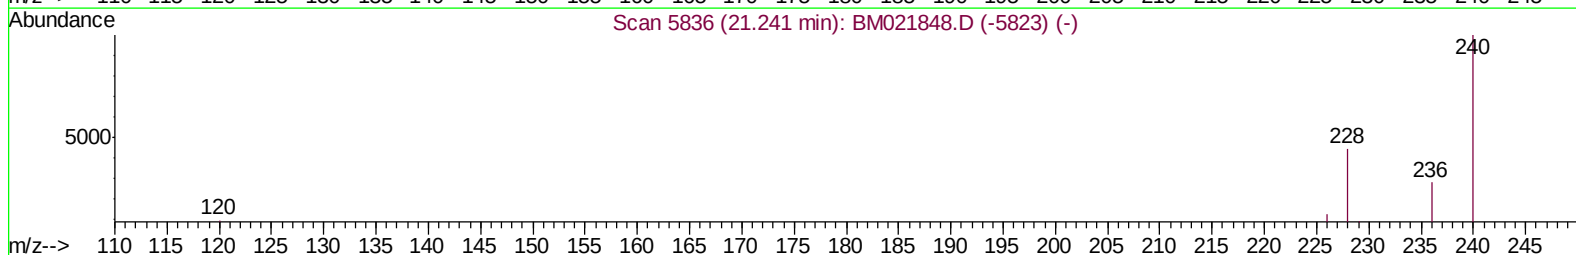
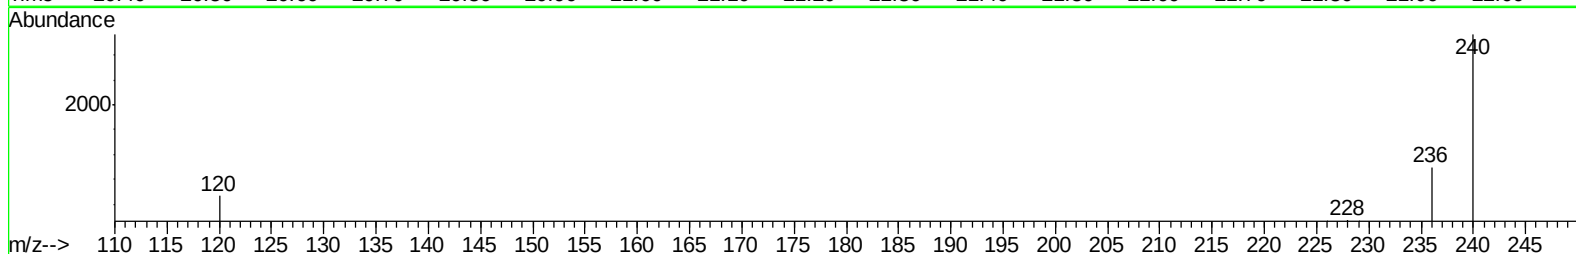


Data File : BM021851.D
Acq On : 05 Aug 2019 20:30
Operator : HP/JU
Sample : K3823-13RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 06 02:00:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

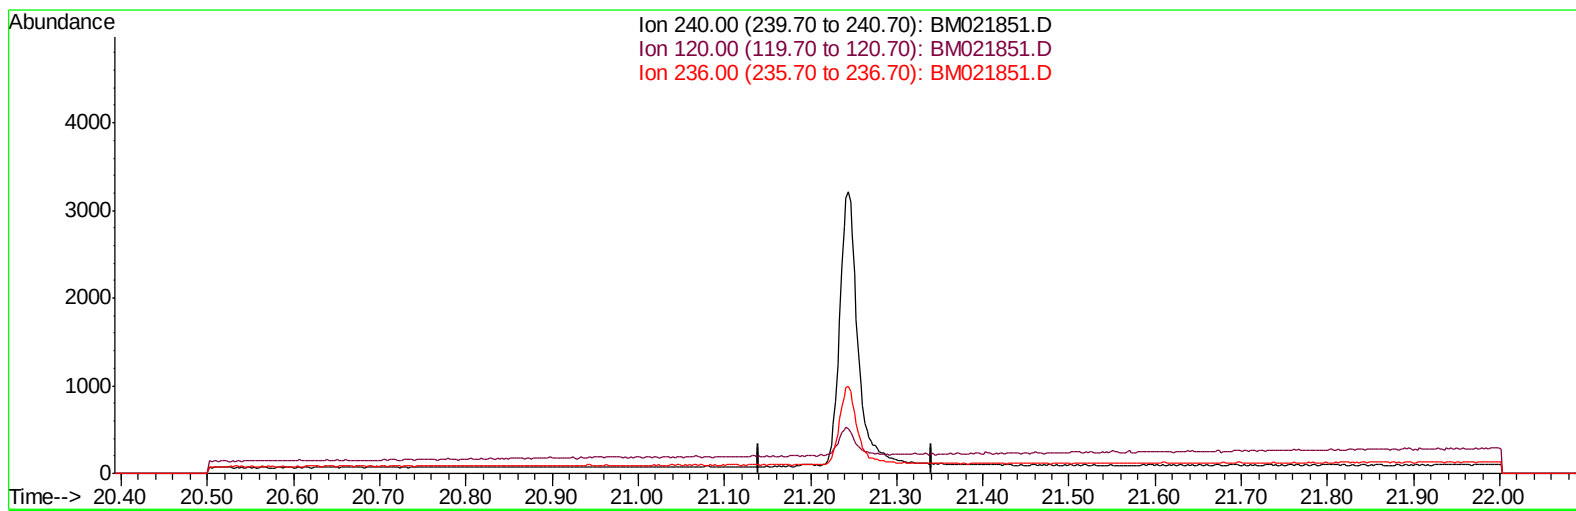

TIC: BM021851.D

(16) Chrysene-d12 (I)

21.241min (-21.241) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	16.20	0.00#
236.00	32.30	0.00#
0.00	0.00	0.00