
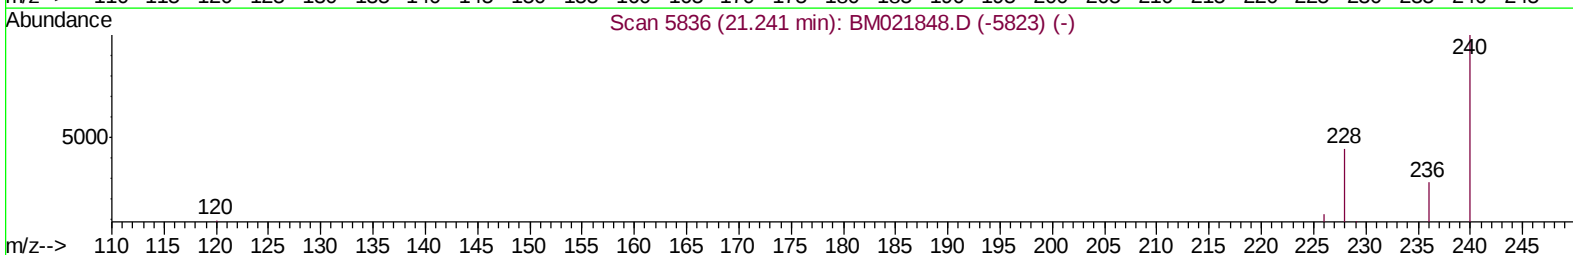
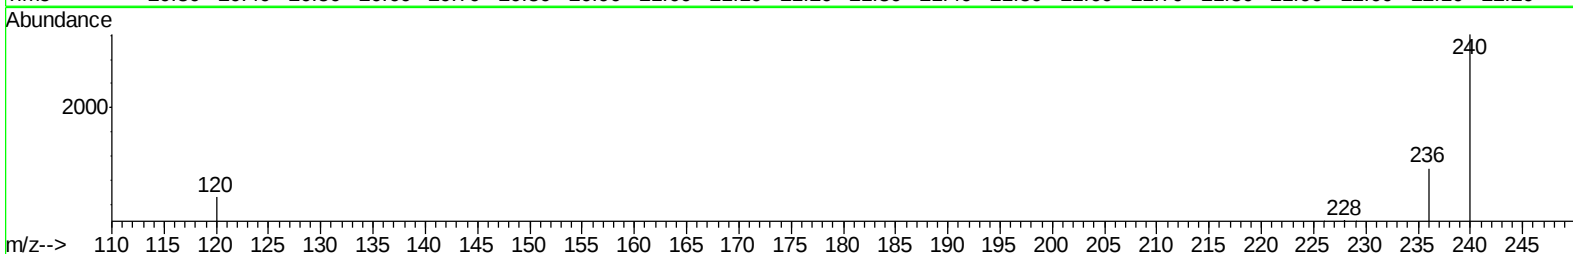


Data File : BM021851.D  
Acq On : 05 Aug 2019 20:30  
Operator : HP/JU  
Sample : K3823-13RE  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 06 02:00:03 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 06 01:29:26 2019  
Response via : Initial Calibration

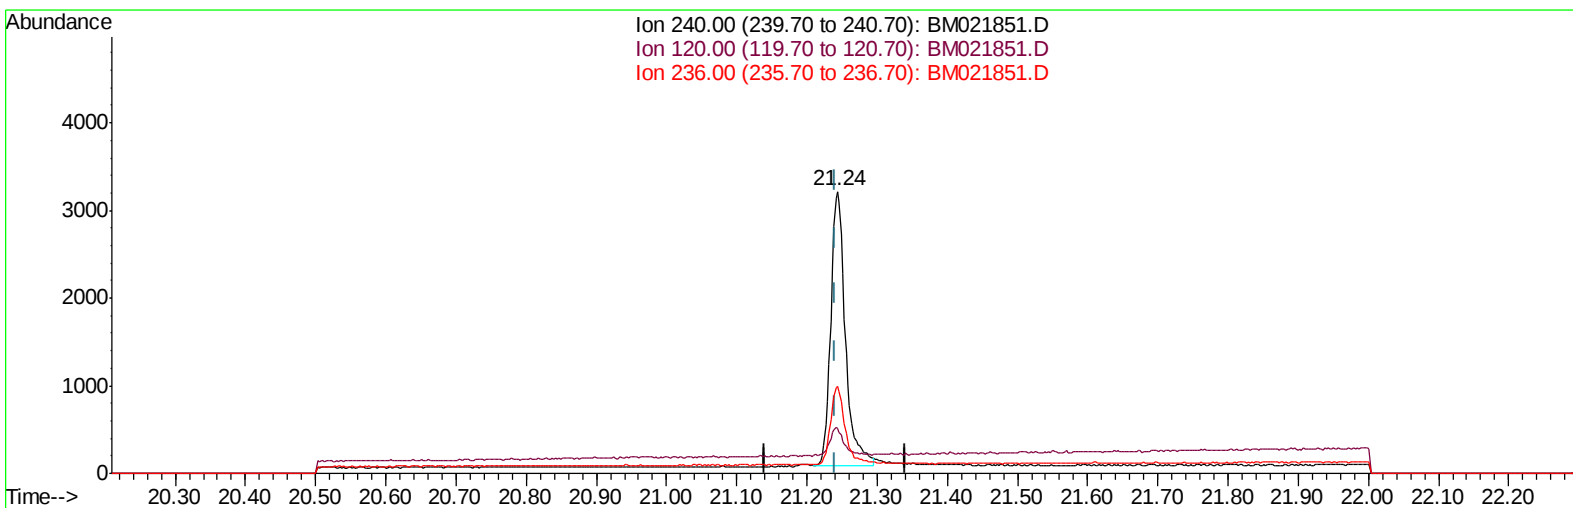

TIC: BM021851.D

(16) Chrysene-d12 (I)

21.244min (+0.002) 0.40ng/ul m

response 4507

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 240.00 | 100   | 100   |
| 120.00 | 16.20 | 16.12 |
| 236.00 | 32.30 | 30.87 |
| 0.00   | 0.00  | 0.00  |