
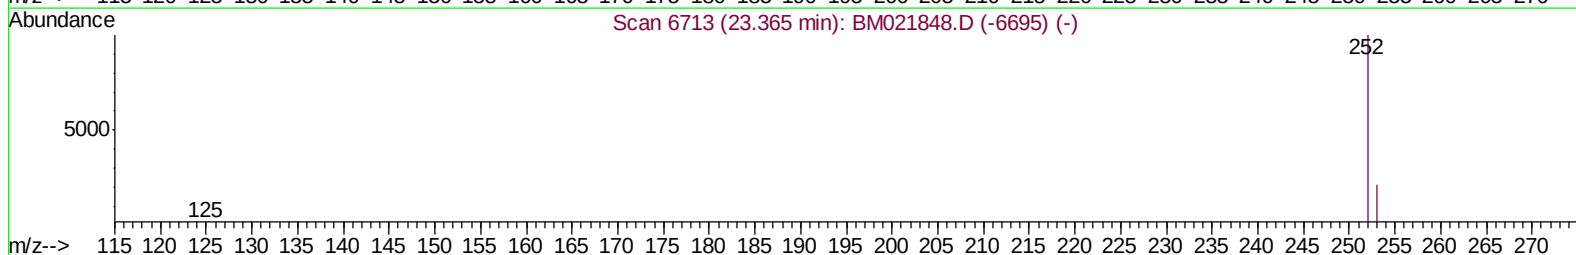
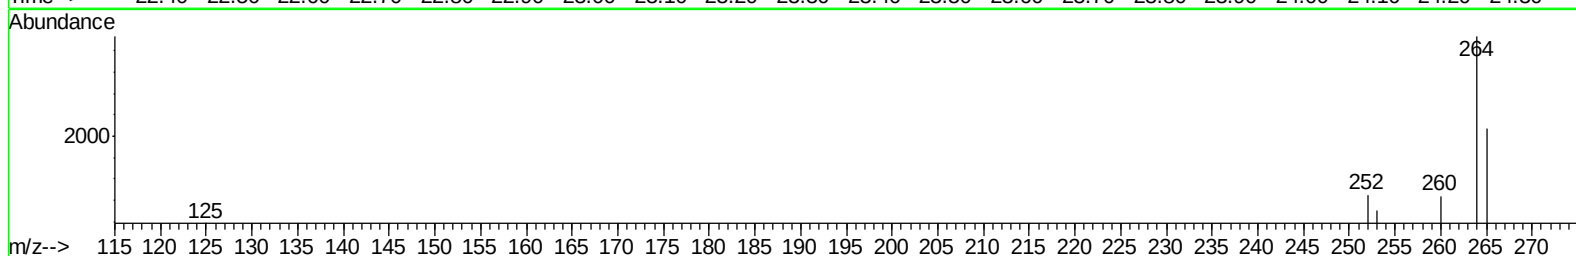


Data File : BM021852.D
Acq On : 05 Aug 2019 21:07
Operator : HP/JU
Sample : K3863-13RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Aug 06 02:10:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

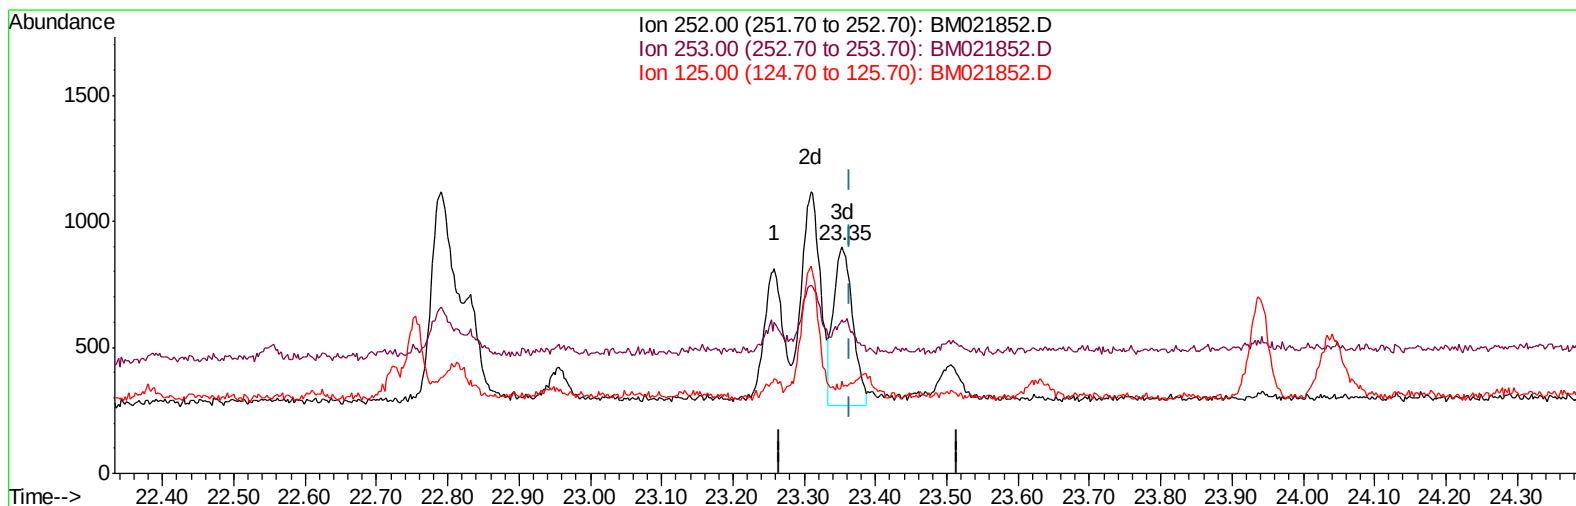

TIC: BM021852.D

(23) Benzo(a)pyrene (C)
23.353min (-0.012) 0.05ng/ul m
response 1165

Ion	Exp%	Act%
252.00	100	100
253.00	39.60	67.74#
125.00	18.20	40.82#
0.00	0.00	0.00