
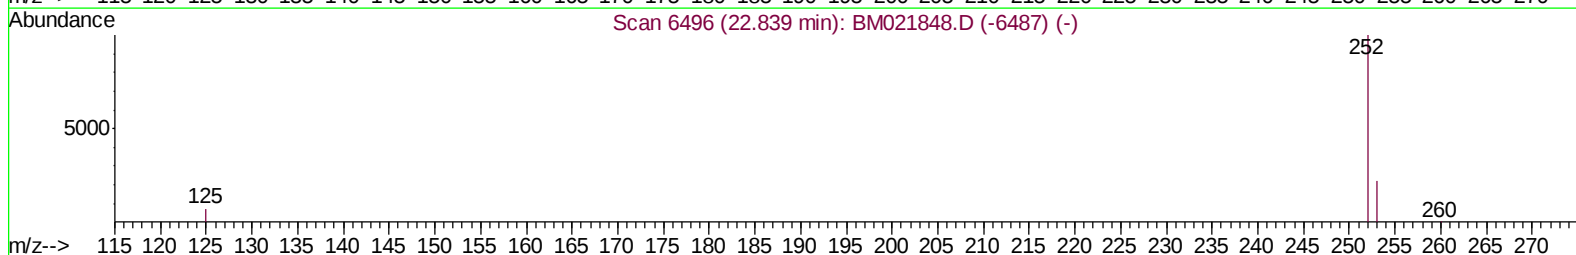
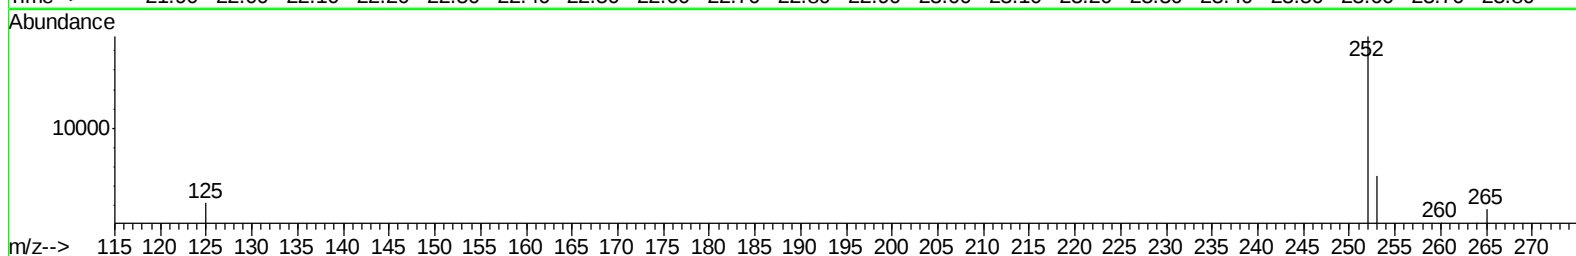


Data File : BM021854.D
Acq On : 05 Aug 2019 22:20
Operator : HP/JU
Sample : K3863-15DL 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 06 02:37:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

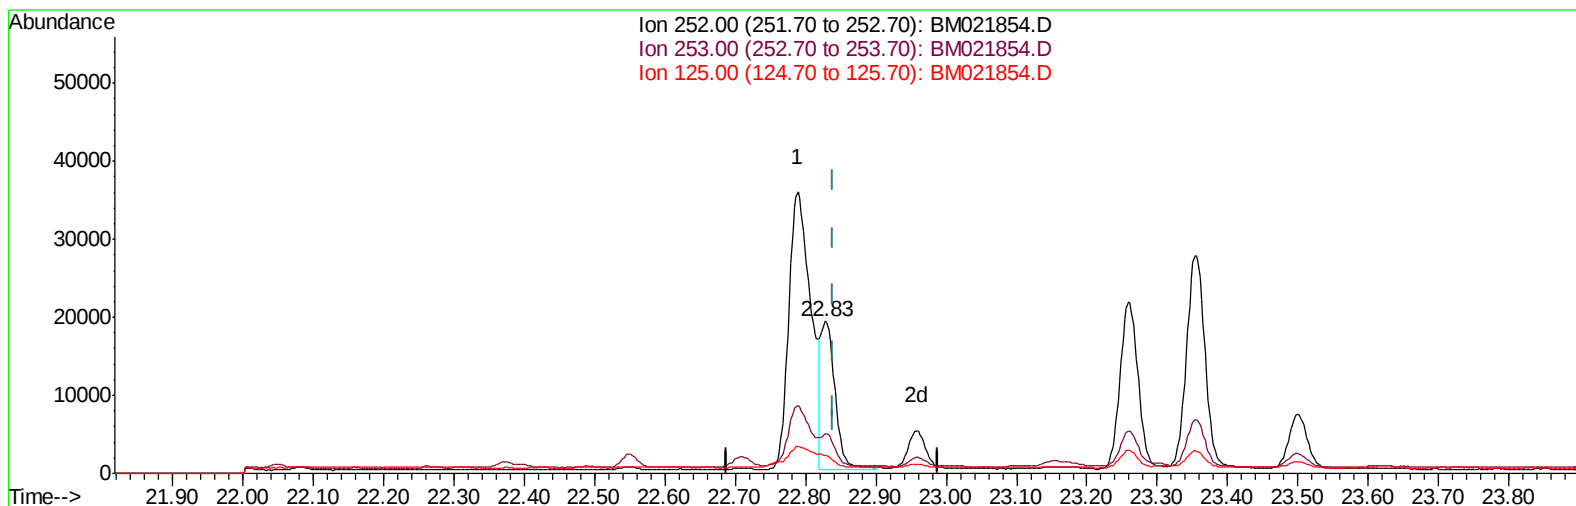

TIC: BM021854.D

(22) Benzo(k)fluoranthene

22.827min (-0.012) 1.35ng/ul m

response 28250

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	25.92#
125.00	15.20	11.91#
0.00	0.00	0.00