
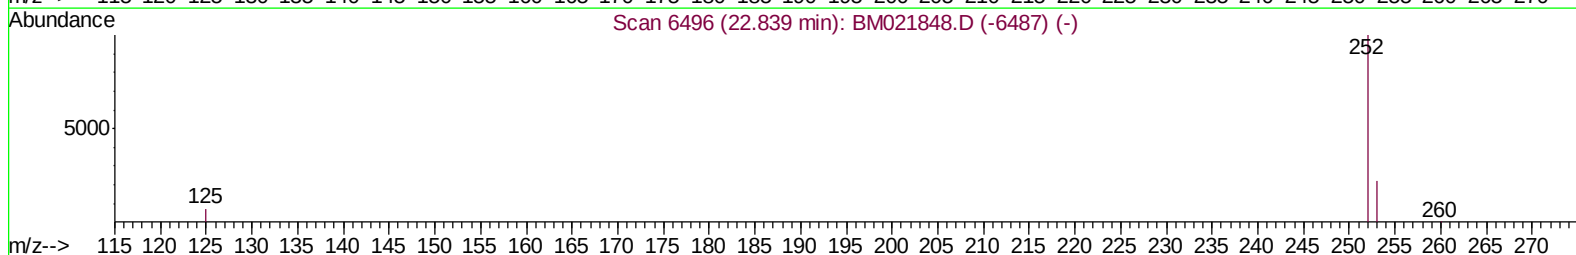
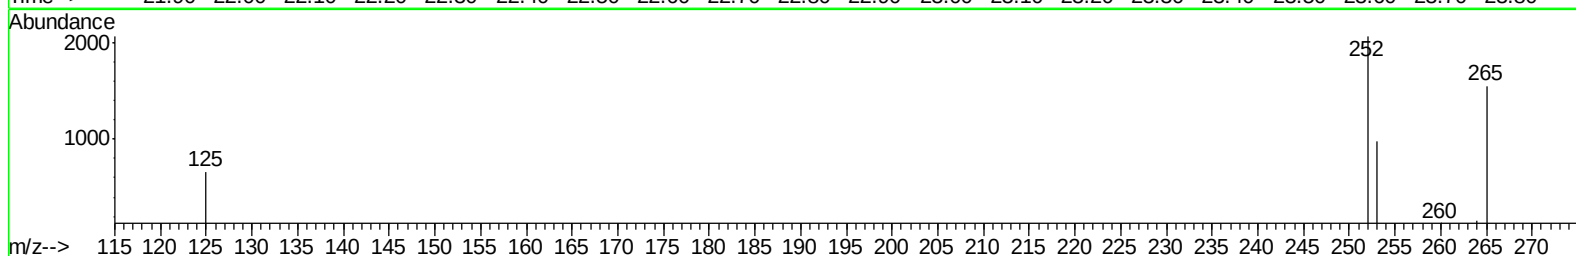


Data File : BM021855.D
Acq On : 05 Aug 2019 22:56
Operator : HP/JU
Sample : K3863-12DL 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 06 01:32:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

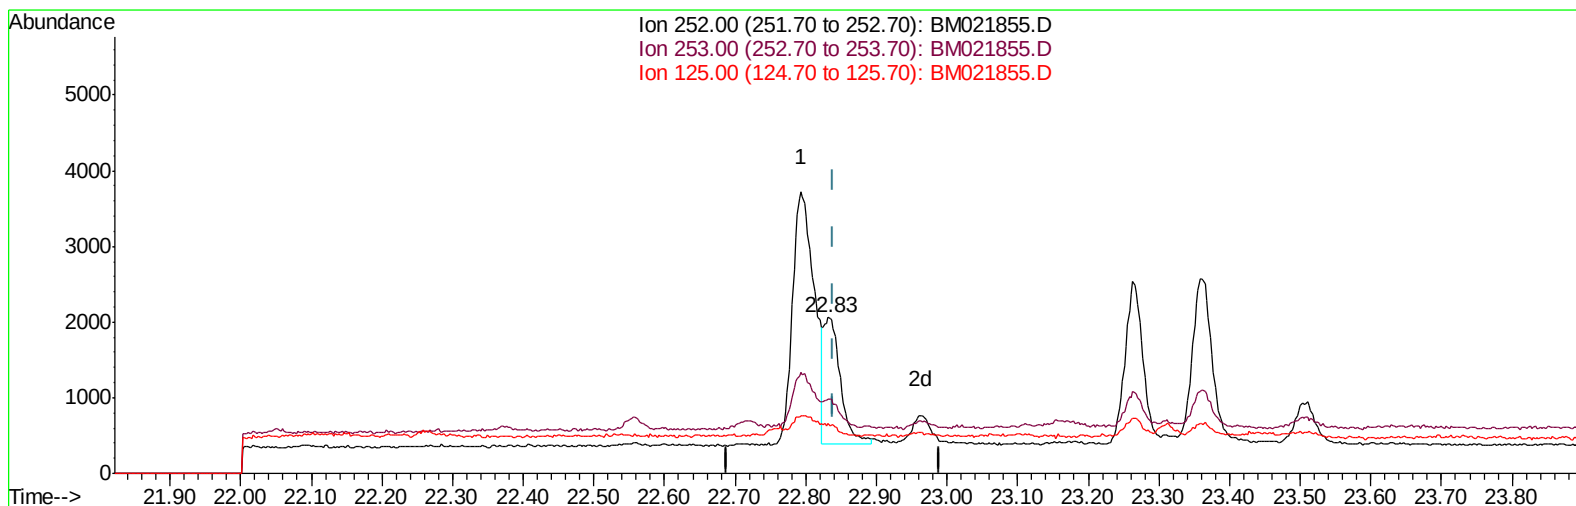

TIC: BM021855.D

(22) Benzo(k)fluoranthene

22.832min (-0.007) 0.13ng/ul m

response 2848

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	47.67#
125.00	15.20	32.18#
0.00	0.00	0.00