
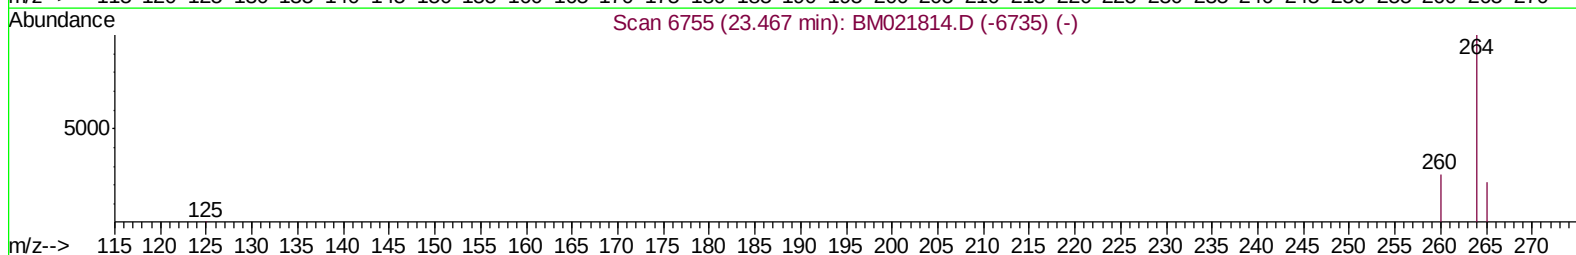
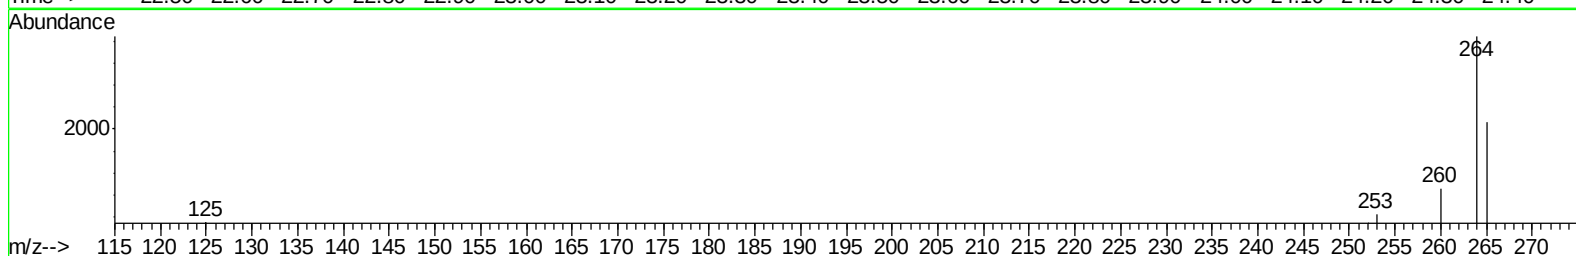


Data File : BM021823.D
Acq On : 04 Aug 2019 21:28
Operator : HP/JU
Sample : K4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Quant Time: Aug 05 08:16:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 06:57:04 2019
Response via : Initial Calibration

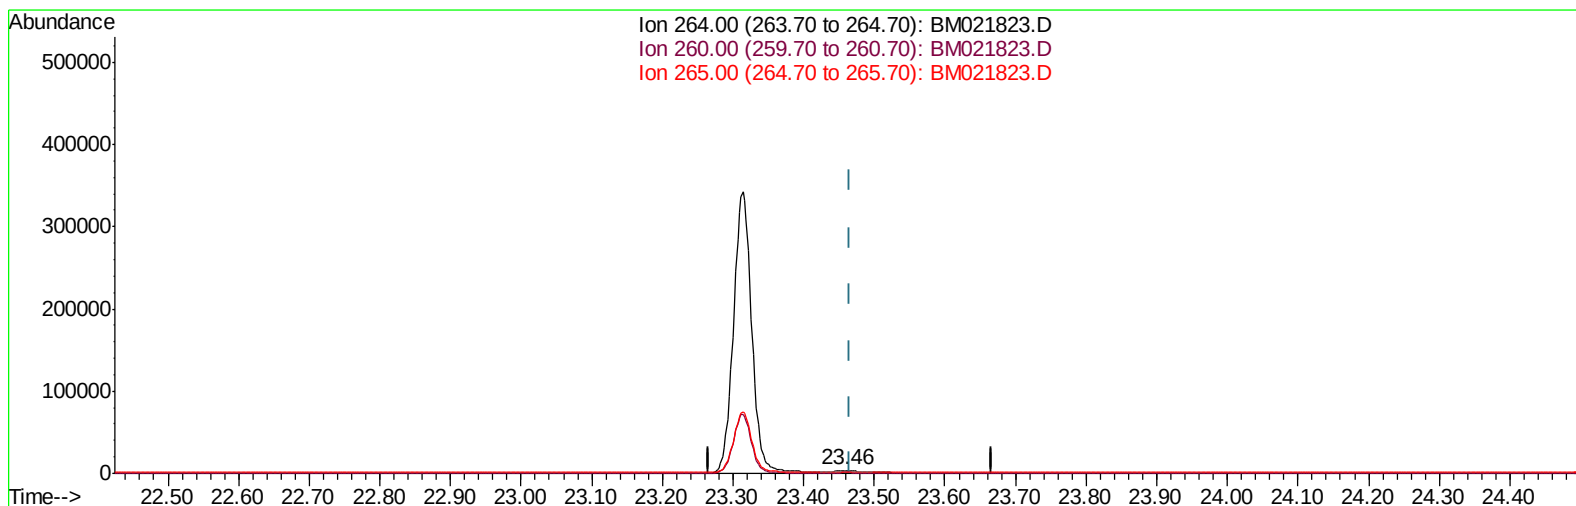

TIC: BM021823.D

(20) Perylene-d12 (I)

23.459min (-0.007) 0.40ng/ul m

response 4371

Ion	Exp%	Act%
264.00	100	100
260.00	27.50	24.83
265.00	117.00	57.62#
0.00	0.00	0.00