
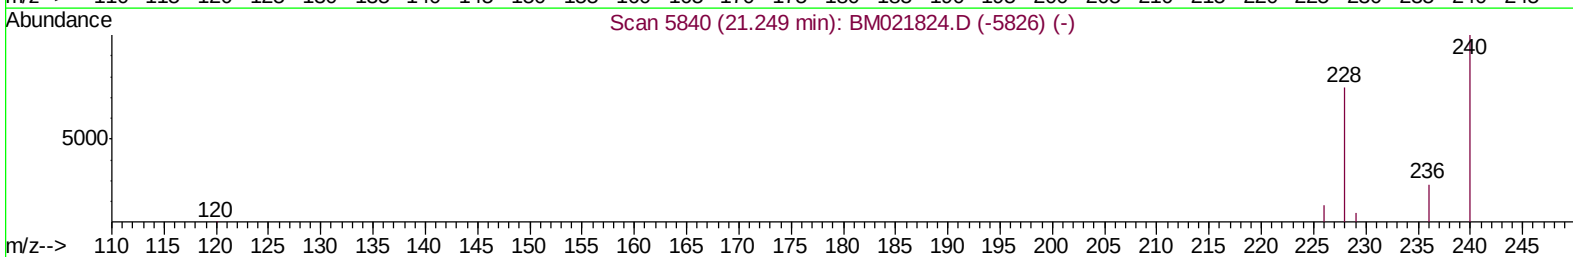
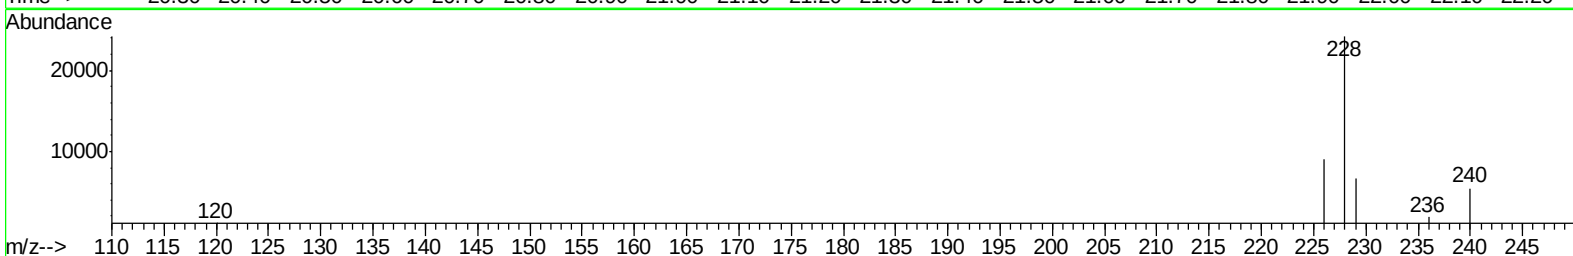


Data File : BM021825.D
Acq On : 04 Aug 2019 23:54
Operator : HP/JU
Sample : K3863-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Aug 05 08:26:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

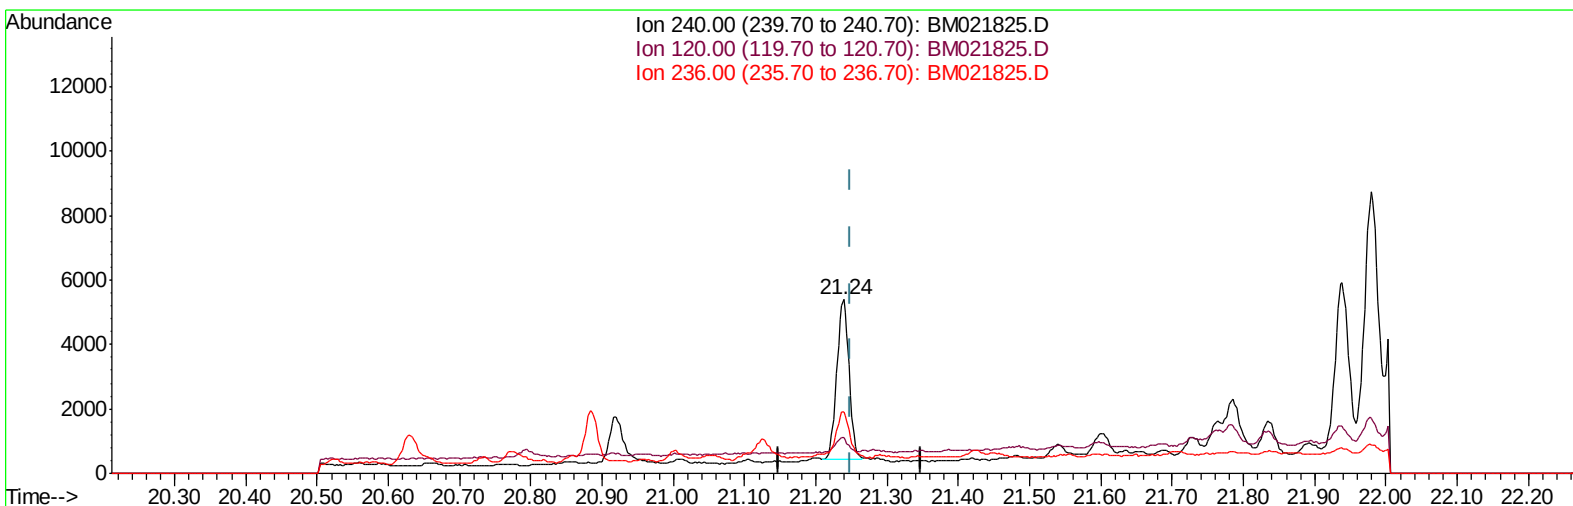

TIC: BM021825.D

(16) Chrysene-d12 (I)

21.239min (-0.010) 0.40ng/ul m

response 6025

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	20.75#
236.00	32.30	35.09
0.00	0.00	0.00