
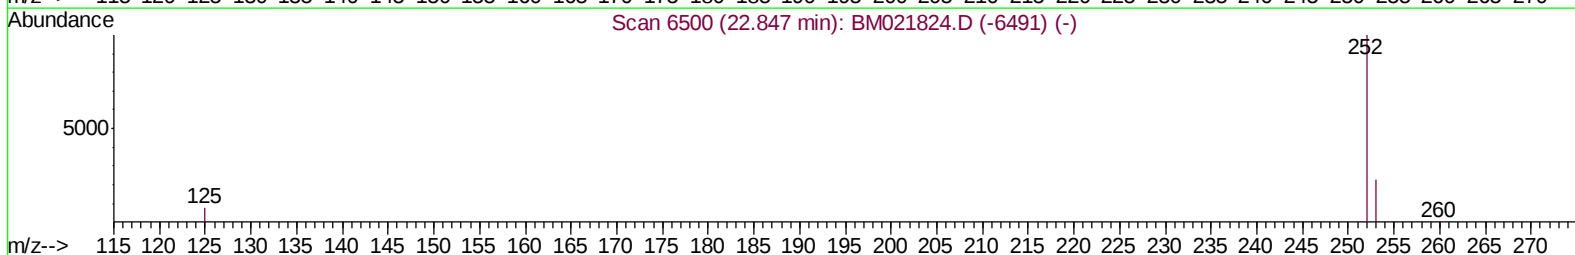
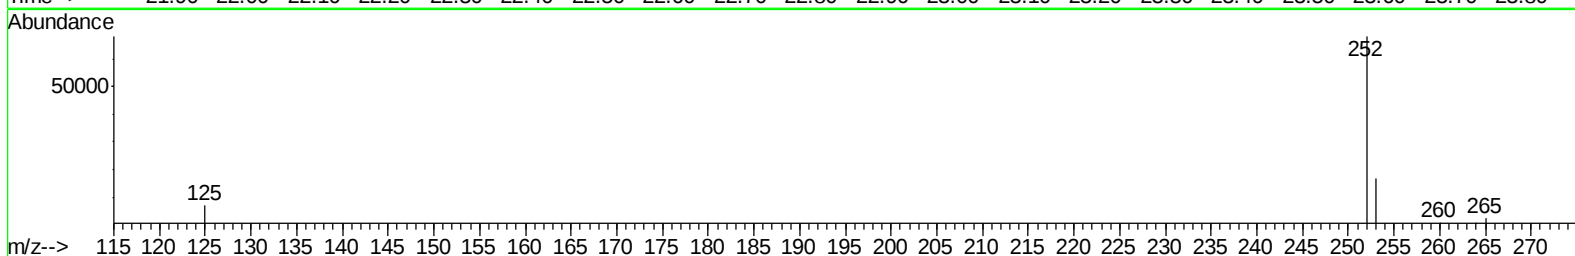


Data File : BM021825.D
Acq On : 04 Aug 2019 23:54
Operator : HP/JU
Sample : K3863-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Aug 05 08:28:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

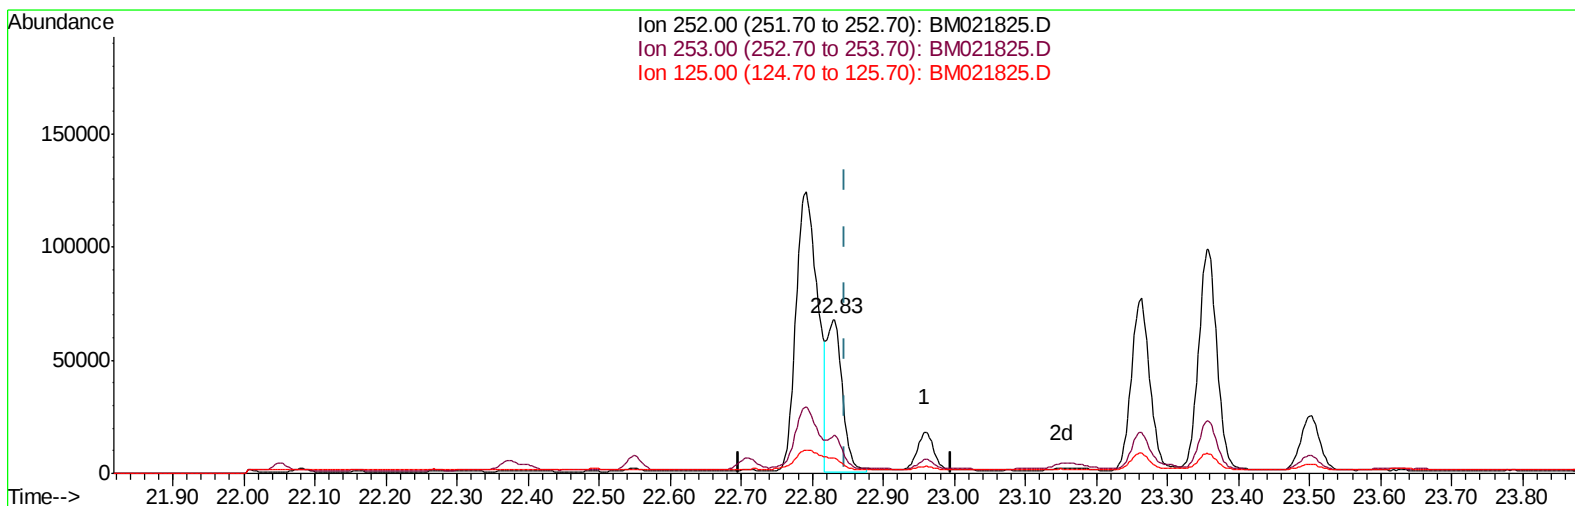

TIC: BM021825.D

(22) Benzo(k)fluoranthene

22.830min (-0.017) 3.83ng/ul m

response 101853

Ion	Exp%	Act%
252.00	100	100
253.00	33.70	24.51#
125.00	15.20	10.05#
0.00	0.00	0.00