
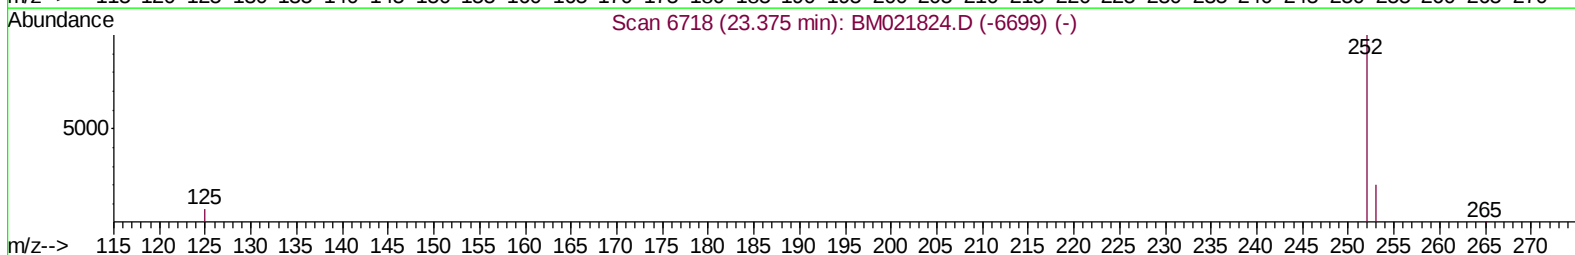
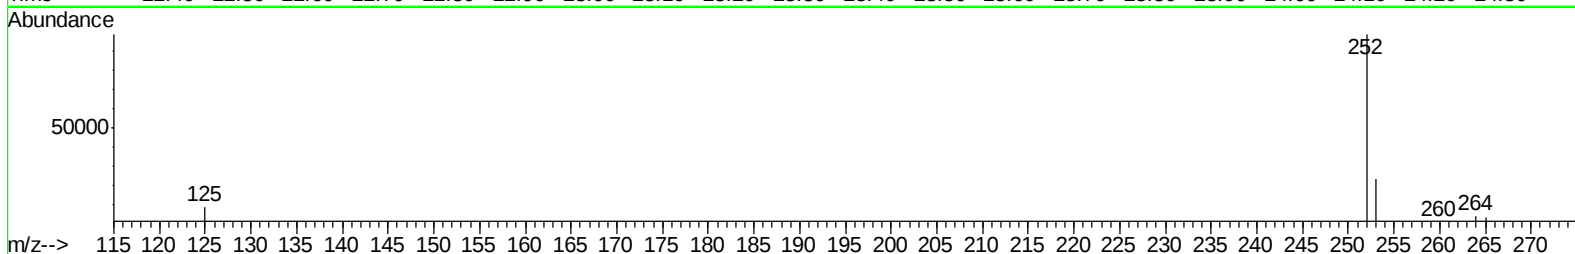


Data File : BM021825.D
Acq On : 04 Aug 2019 23:54
Operator : HP/JU
Sample : K3863-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Aug 05 08:28:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

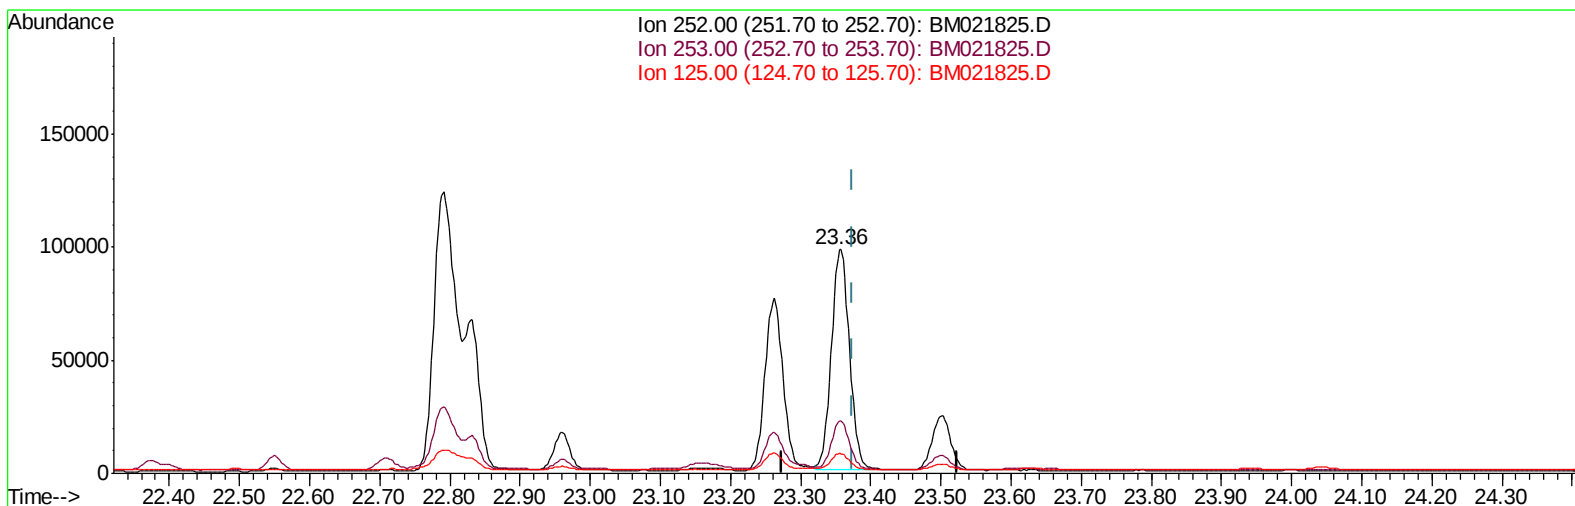

TIC: BM021825.D

(23) Benzo(a)pyrene (C)
23.355min (-0.020) 7.31ng/ul m
response 174383

Ion	Exp%	Act%
252.00	100	100
253.00	39.60	23.50#
125.00	18.20	8.98#
0.00	0.00	0.00