
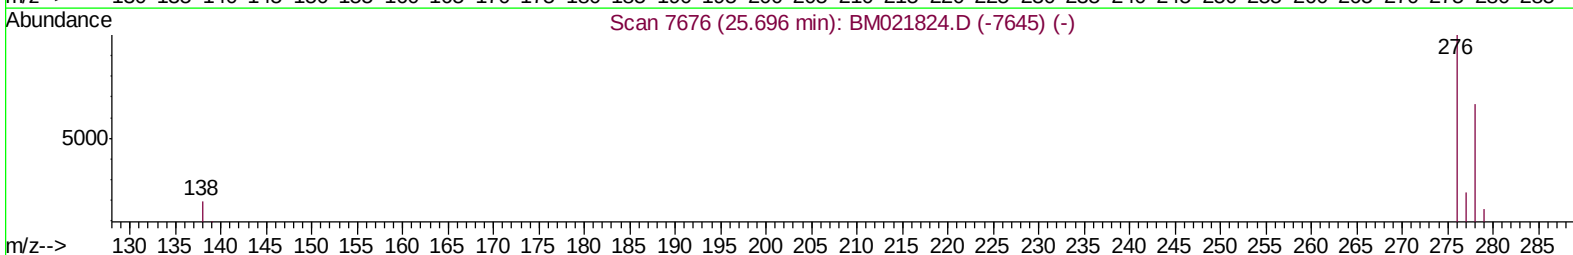
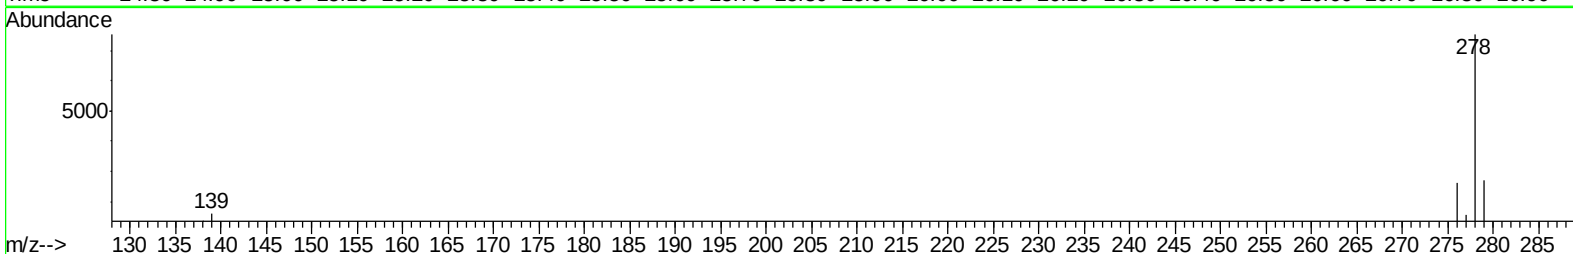


Data File : BM021825.D
Acq On : 04 Aug 2019 23:54
Operator : HP/JU
Sample : K3863-14
Misc :
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Aug 05 08:28:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

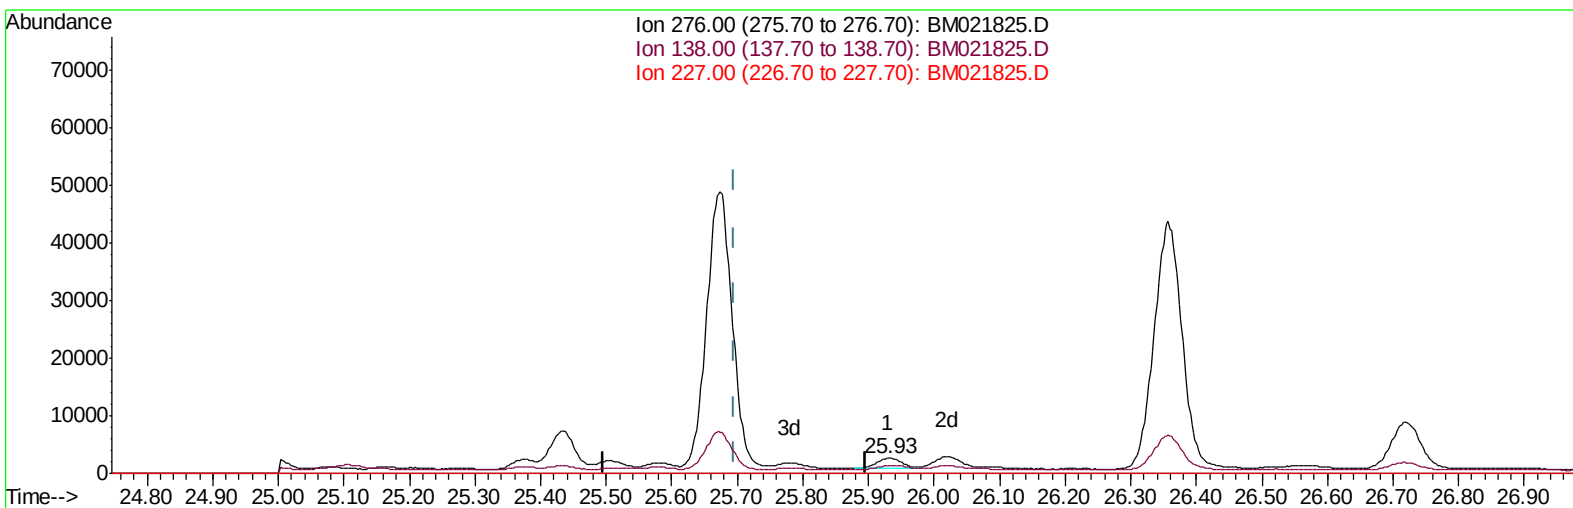

TIC: BM021825.D

(24) Indeno(1,2,3-cd)pyrene

25.931min (+0.235) 0.18ng/ul

response 5156

Ion	Exp%	Act%
276.00	100	100
138.00	18.90	51.26#
227.00	0.00	0.00
0.00	0.00	0.00