
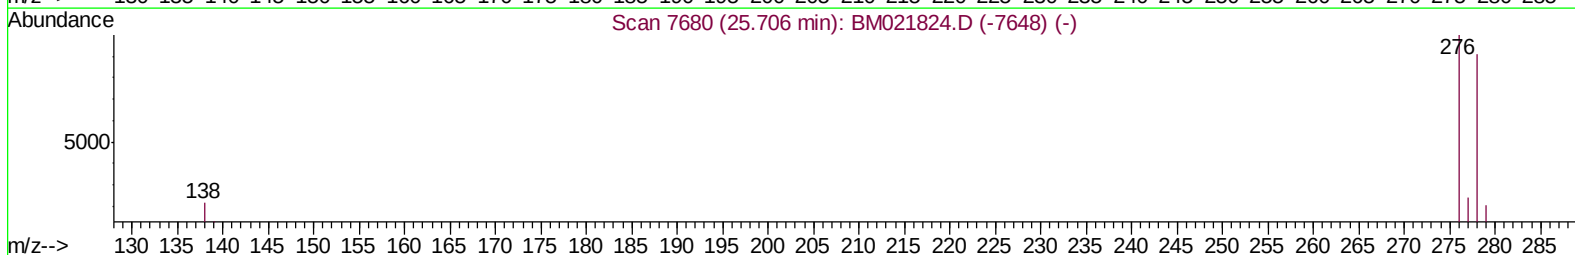
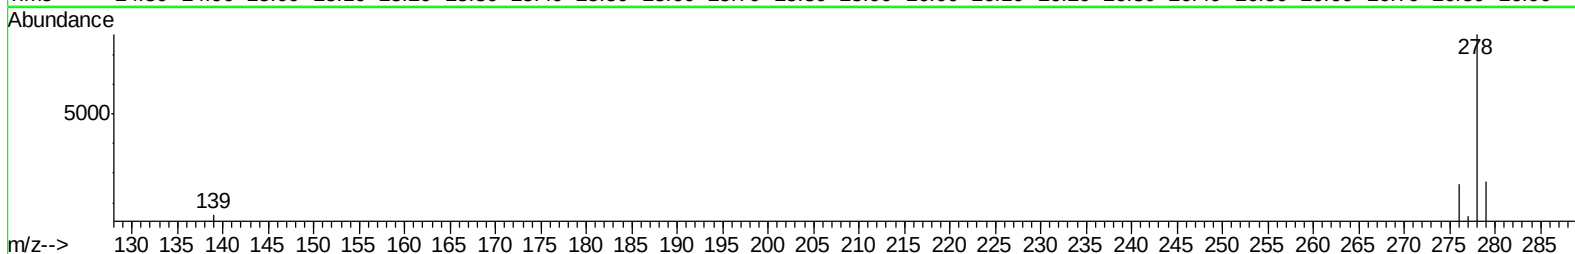


Data File : BM021825.D  
Acq On : 04 Aug 2019 23:54  
Operator : HP/JU  
Sample : K3863-14  
Misc :  
ALS Vial : 68 Sample Multiplier: 1

Quant Time: Aug 05 08:28:34 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

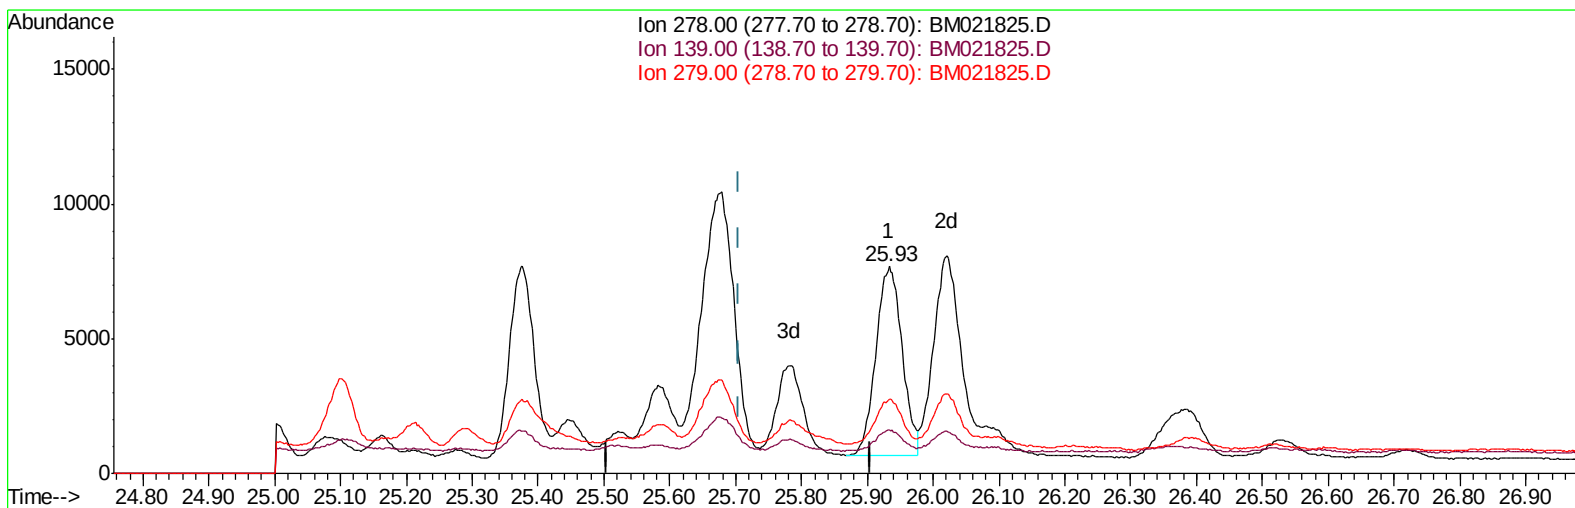

TIC: BM021825.D

(25) Dibenzo(a,h)anthracene

25.933min (+0.228) 0.84ng/ul

response 19396

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 278.00 | 100   | 100   |
| 139.00 | 17.70 | 21.04 |
| 279.00 | 35.40 | 35.64 |
| 0.00   | 0.00  | 0.00  |