
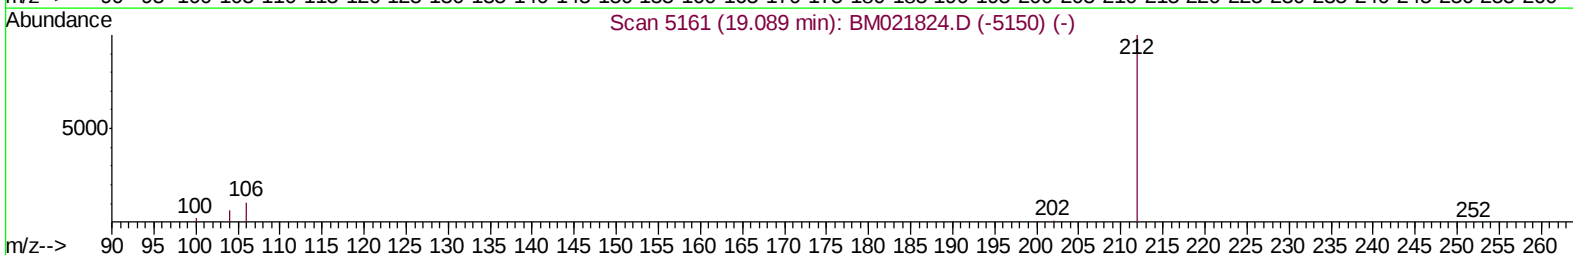
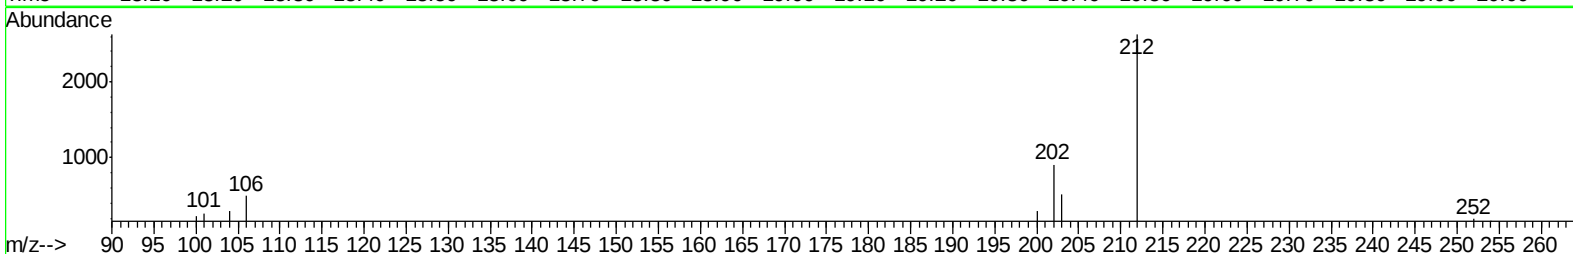


Data File : BM021826.D
Acq On : 05 Aug 2019 00:30
Operator : HP/JU
Sample : K3863-15
Misc :
ALS Vial : 69 Sample Multiplier: 1

Quant Time: Aug 05 08:31:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

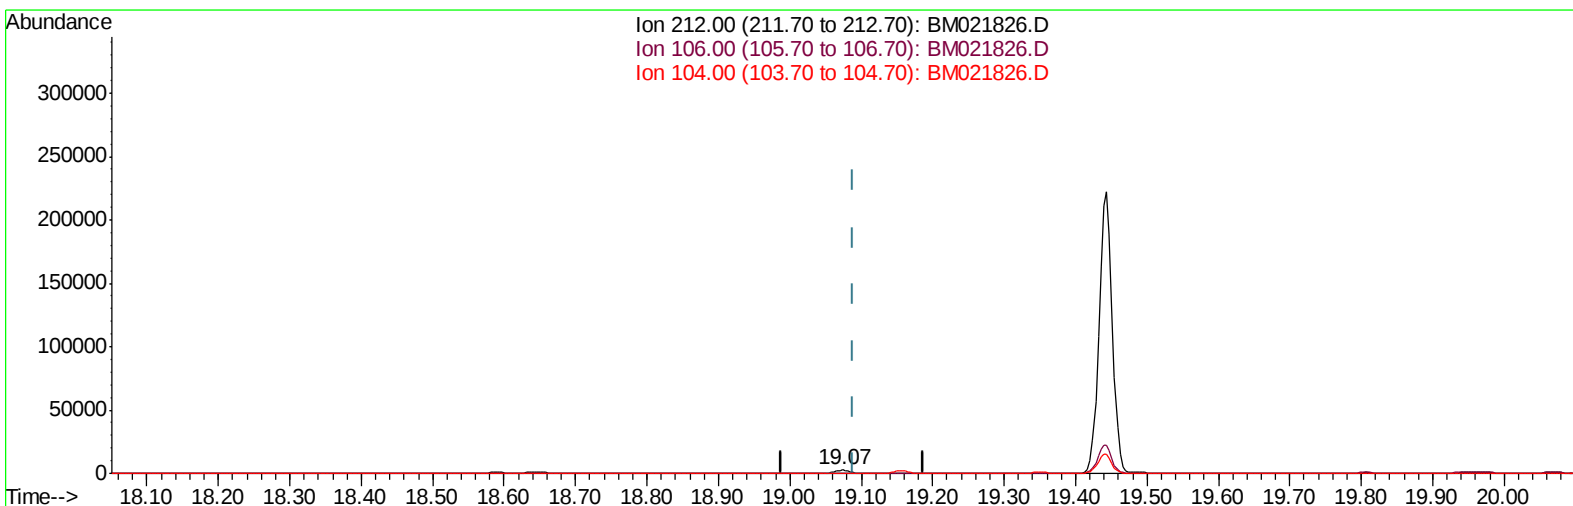

TIC: BM021826.D

(14) Fluoranthene-d10 (SURR)

19.073min (-0.015) 0.21ng/ul m

response 3824

Ion	Exp%	Act%
212.00	100	100
106.00	9.90	0.65#
104.00	6.00	66.95#
0.00	0.00	0.00