
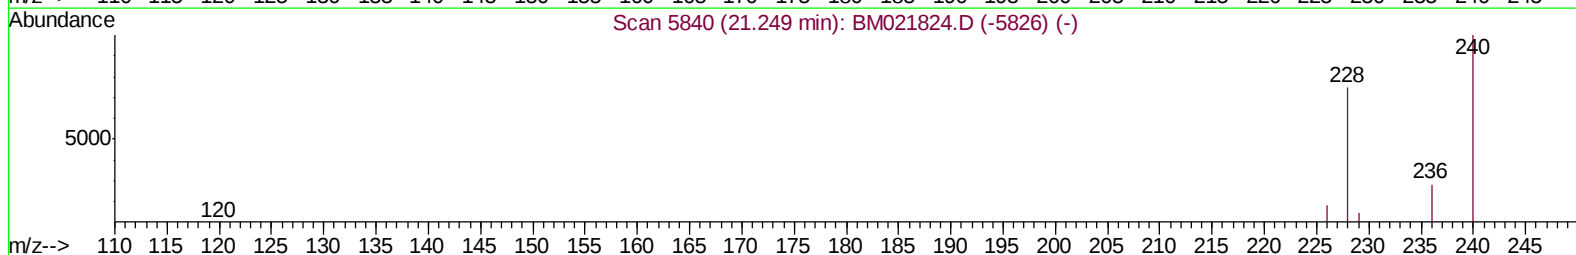
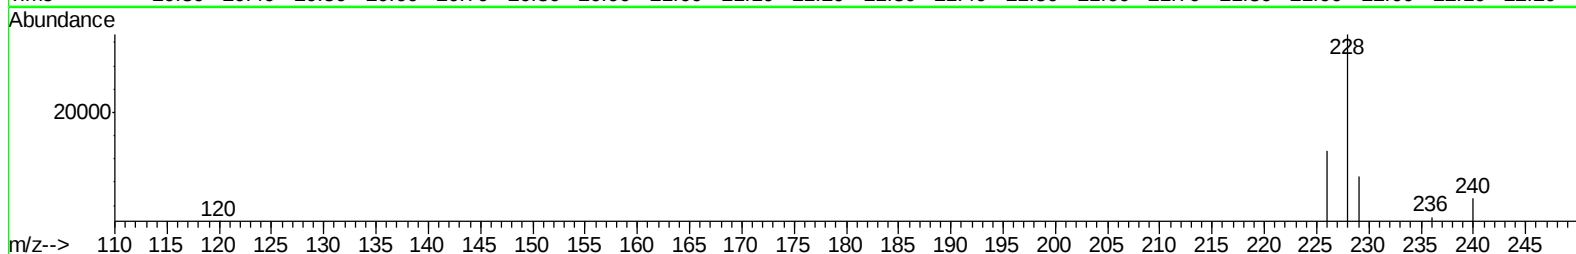


Data File : BM021826.D
Acq On : 05 Aug 2019 00:30
Operator : HP/JU
Sample : K3863-15
Misc :
ALS Vial : 69 Sample Multiplier: 1

Quant Time: Aug 05 08:31:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

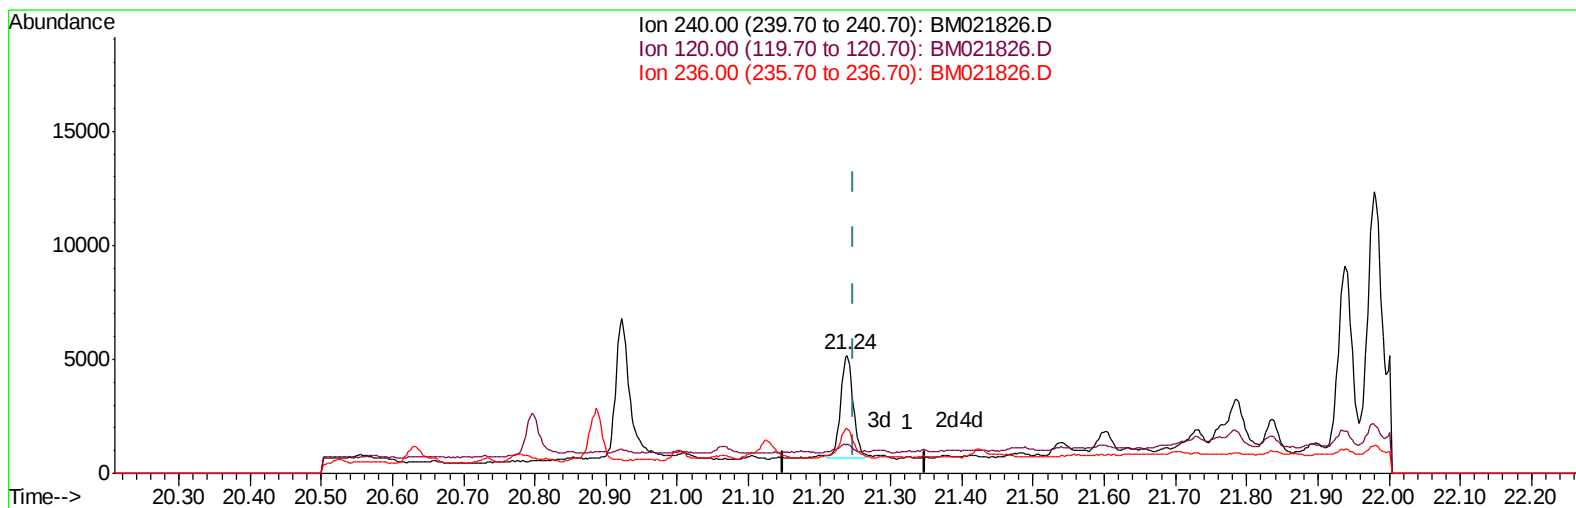

TIC: BM021826.D

(16) Chrysene-d12 (I)

21.239min (-0.010) 0.40ng/ul m

response 5494

Ion	Exp%	Act%
240.00	100	100
120.00	16.20	24.50#
236.00	32.30	38.03
0.00	0.00	0.00