
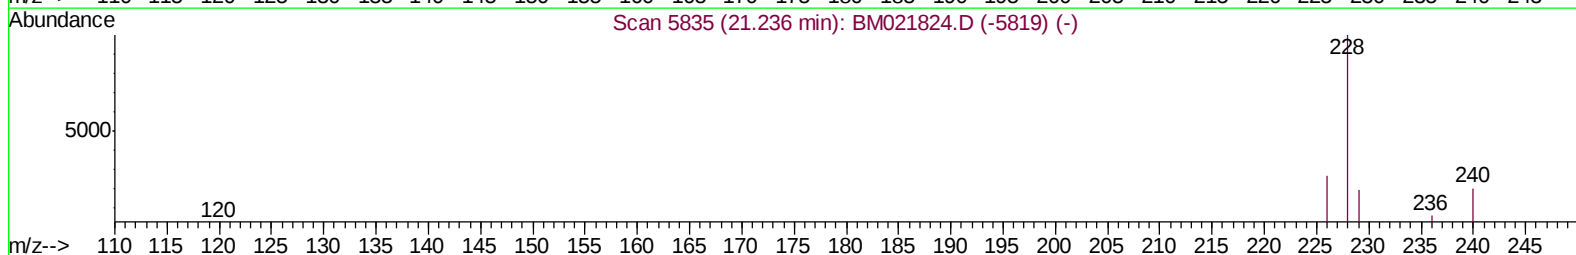
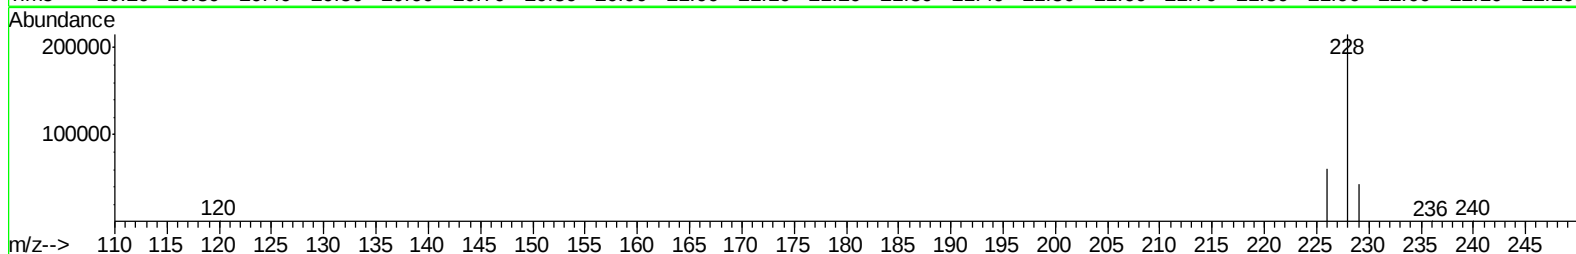


Data File : BM021826.D
Acq On : 05 Aug 2019 00:30
Operator : HP/JU
Sample : K3863-15
Misc :
ALS Vial : 69 Sample Multiplier: 1

Quant Time: Aug 05 08:32:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

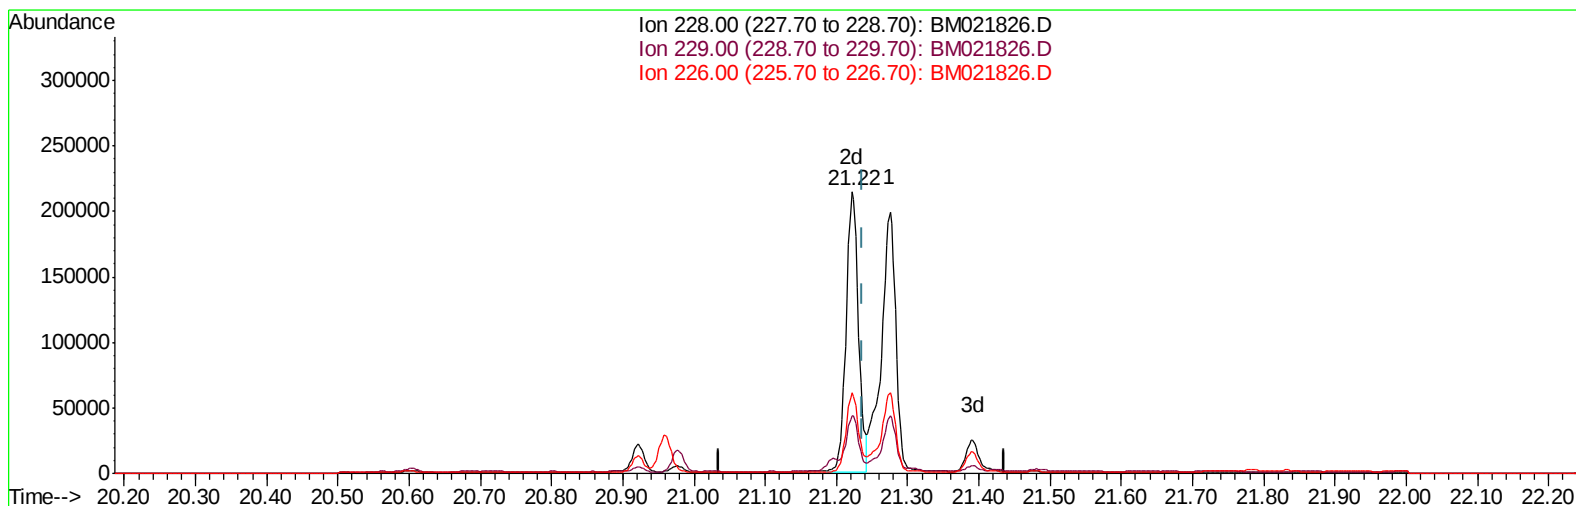

TIC: BM021826.D

(18) Benzo(a)anthracene
21.222min (-0.014) 13.17ng/ul m
response 258841

Ion	Exp%	Act%
228.00	100	100
229.00	21.50	20.56
226.00	28.30	28.56
0.00	0.00	0.00