
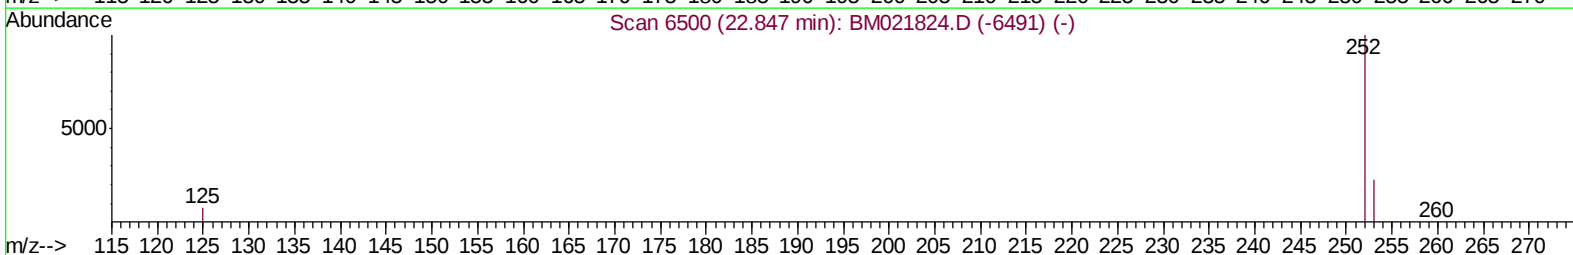
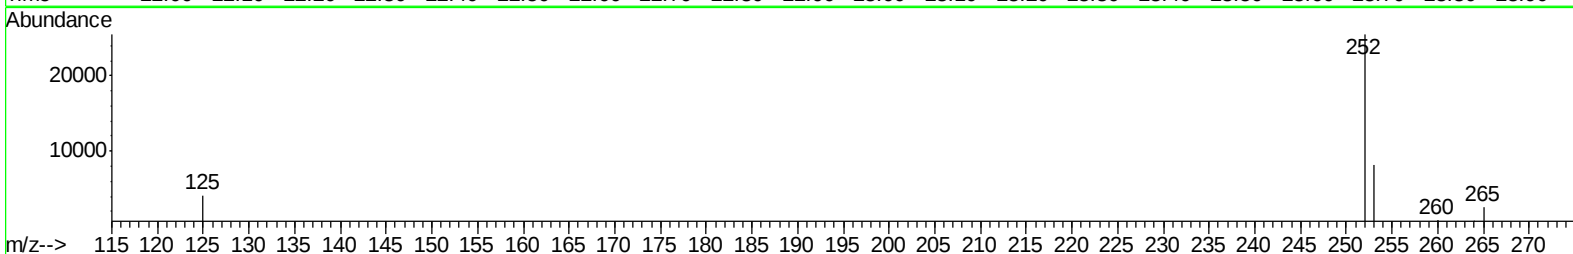


Data File : BM021826.D  
Acq On : 05 Aug 2019 00:30  
Operator : HP/JU  
Sample : K3863-15  
Misc :  
ALS Vial : 69 Sample Multiplier: 1

Quant Time: Aug 05 08:32:20 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

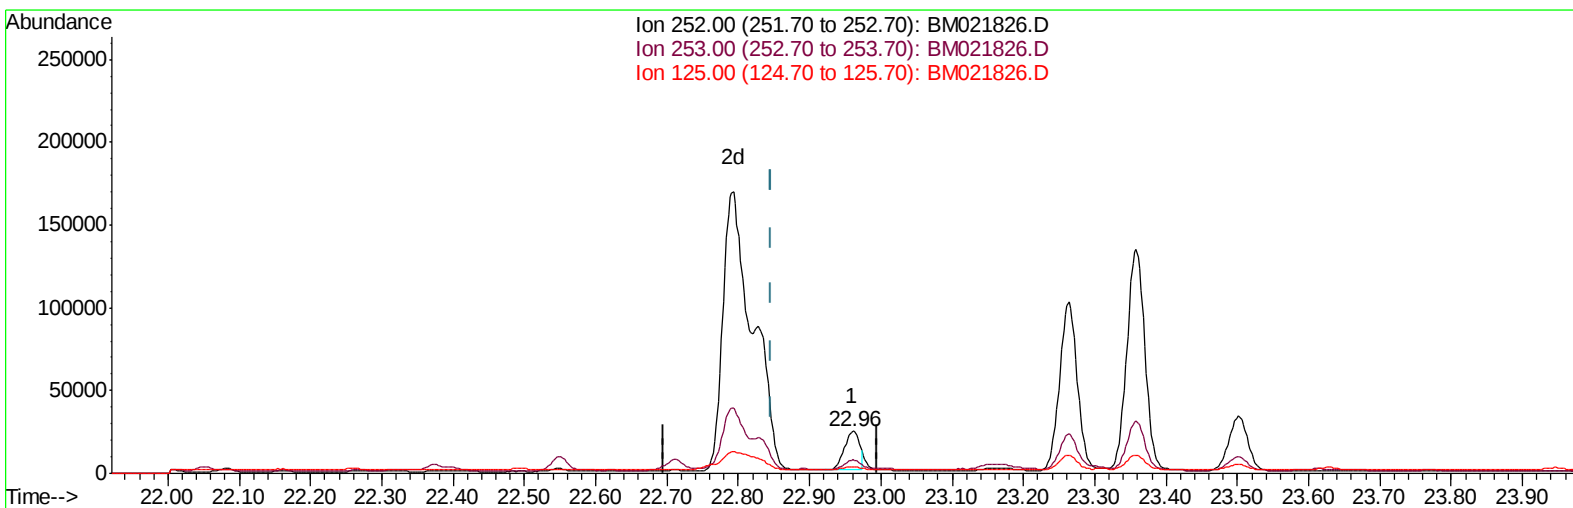

TIC: BM021826.D

(22) Benzo(k)fluoranthene  
22.961min (+0.114) 1.55ng/ul  
response 34719

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 33.70 | 32.24 |
| 125.00 | 15.20 | 16.27 |
| 0.00   | 0.00  | 0.00  |