
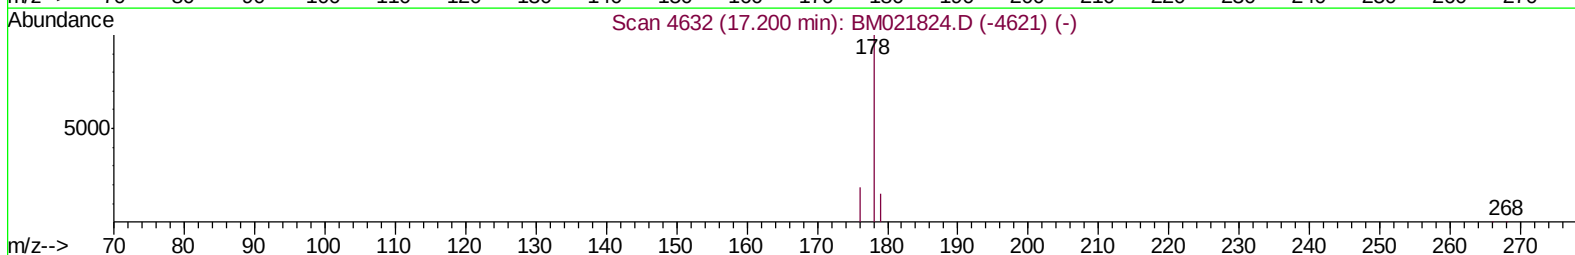
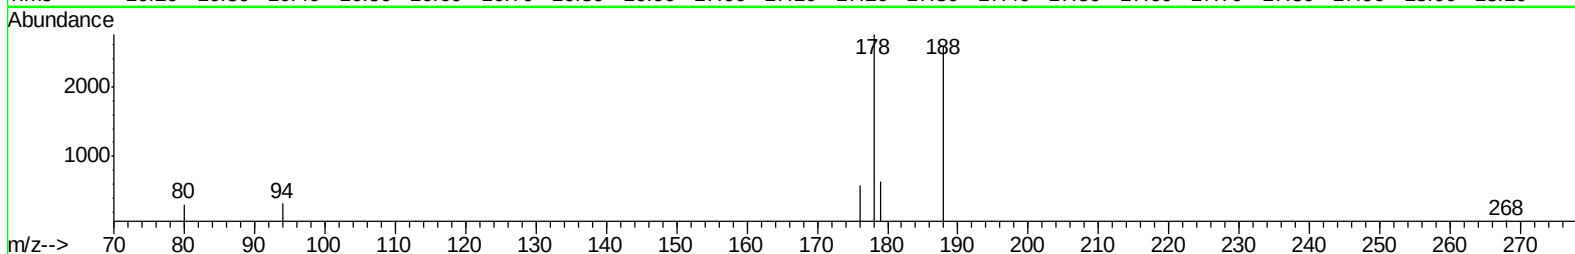


Data File : BM021827.D  
Acq On : 05 Aug 2019 01:06  
Operator : HP/JU  
Sample : K3863-12  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Quant Time: Aug 05 08:39:37 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

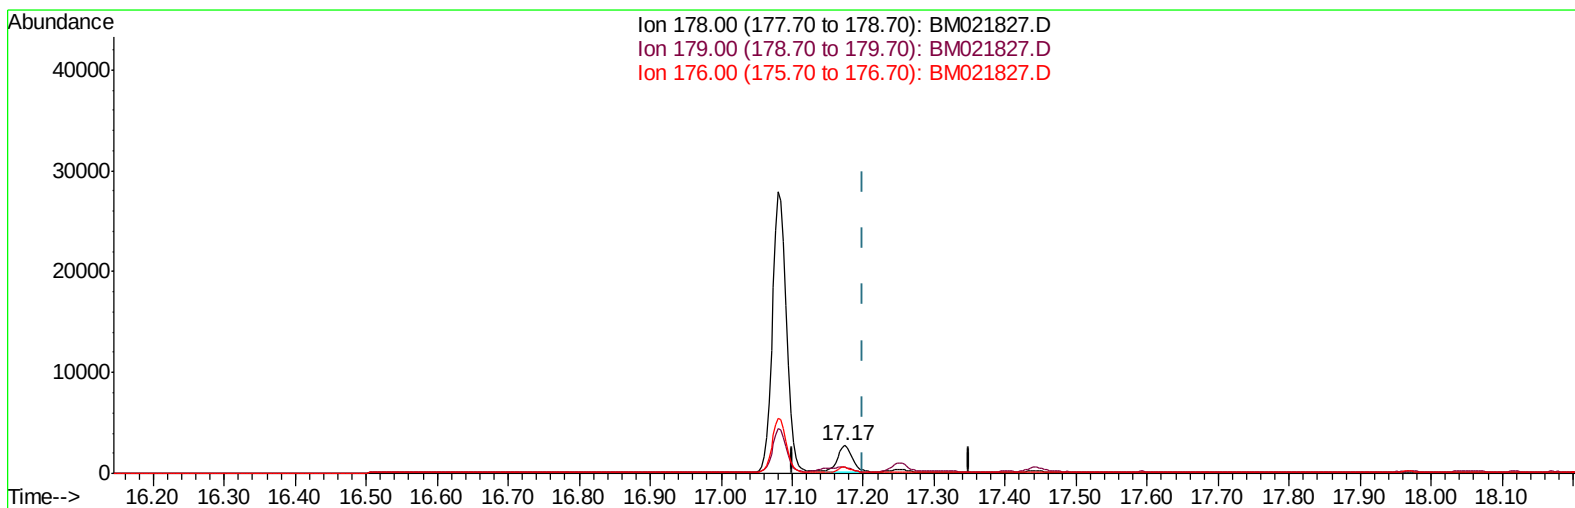

TIC: BM021827.D

(13) Anthracene

17.174min (-0.026) 0.21ng/ul m

response 3773

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 178.00 | 100   | 100   |
| 179.00 | 19.40 | 23.09 |
| 176.00 | 20.80 | 21.34 |
| 0.00   | 0.00  | 0.00  |