
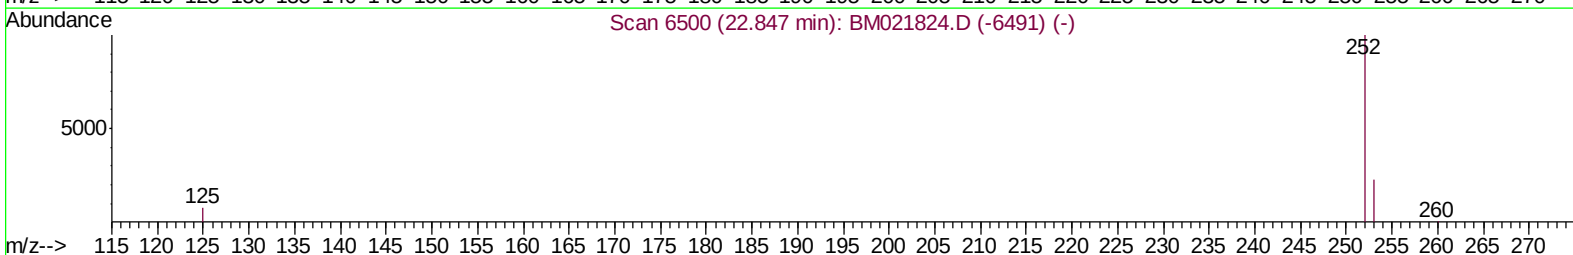
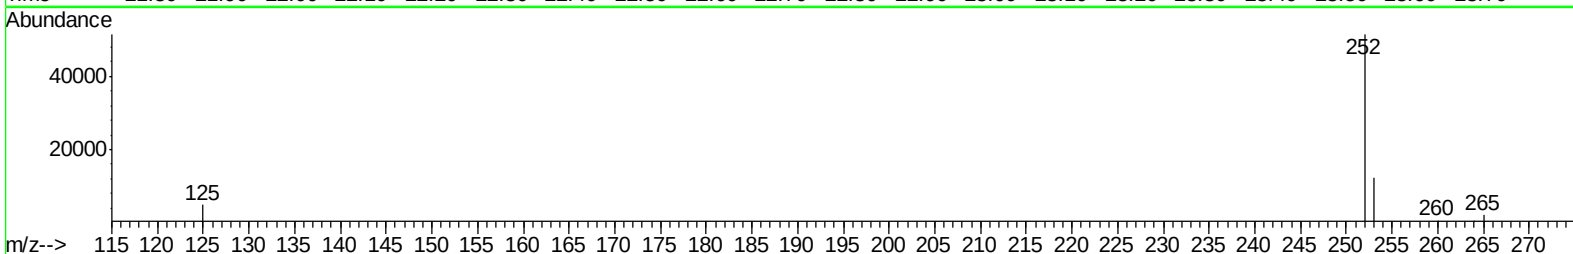


Data File : BM021827.D  
Acq On : 05 Aug 2019 01:06  
Operator : HP/JU  
Sample : K3863-12  
Misc :  
ALS Vial : 70 Sample Multiplier: 1

Quant Time: Aug 05 08:41:12 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

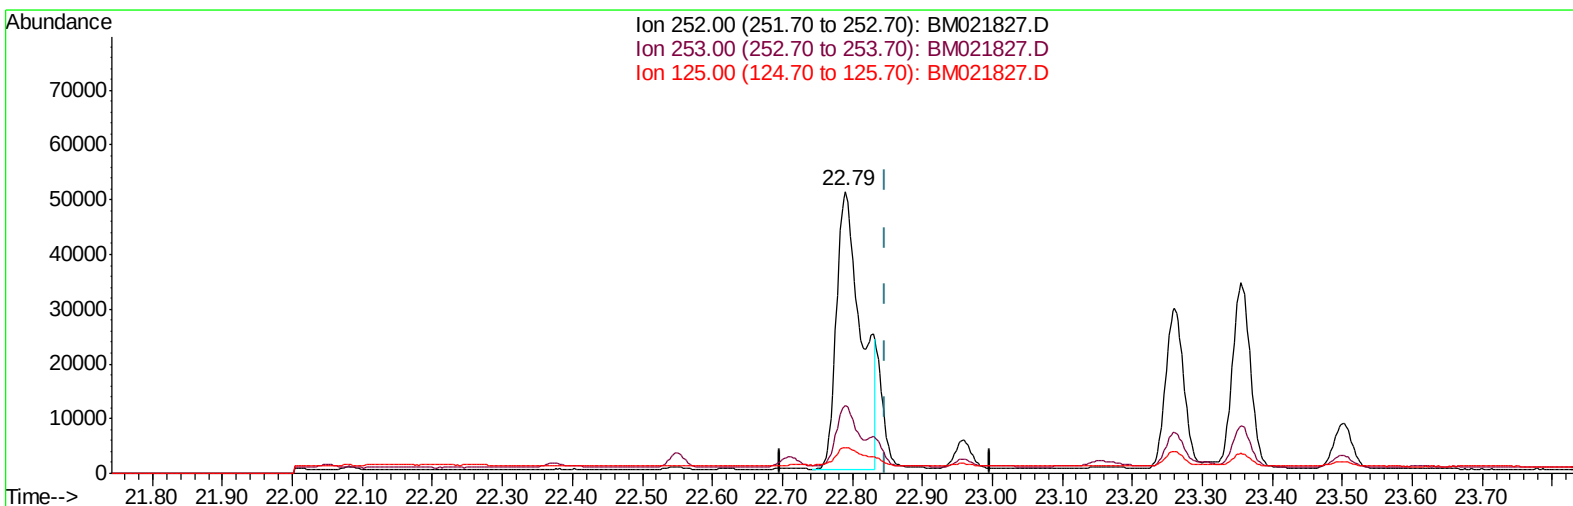

TIC: BM021827.D

(22) Benzo(k)fluoranthene  
22.791min (-0.056) 3.88ng/ul  
response 122711

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 33.70 | 24.10# |
| 125.00 | 15.20 | 9.31#  |
| 0.00   | 0.00  | 0.00   |