
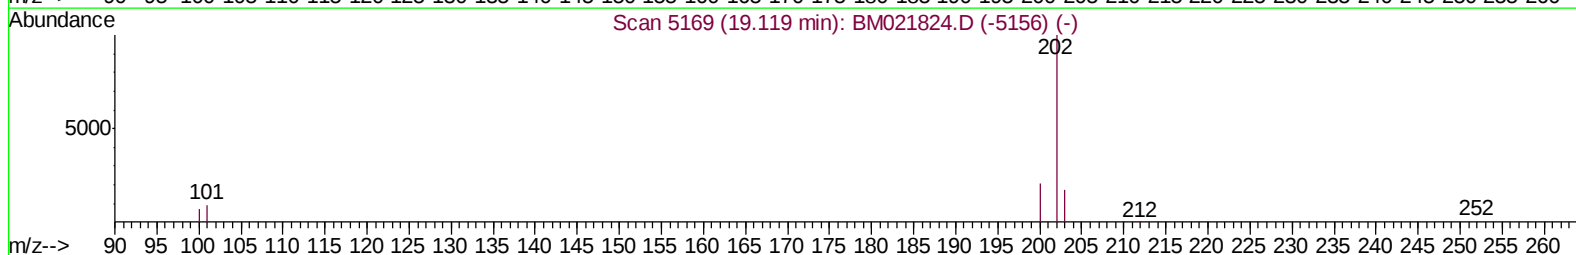
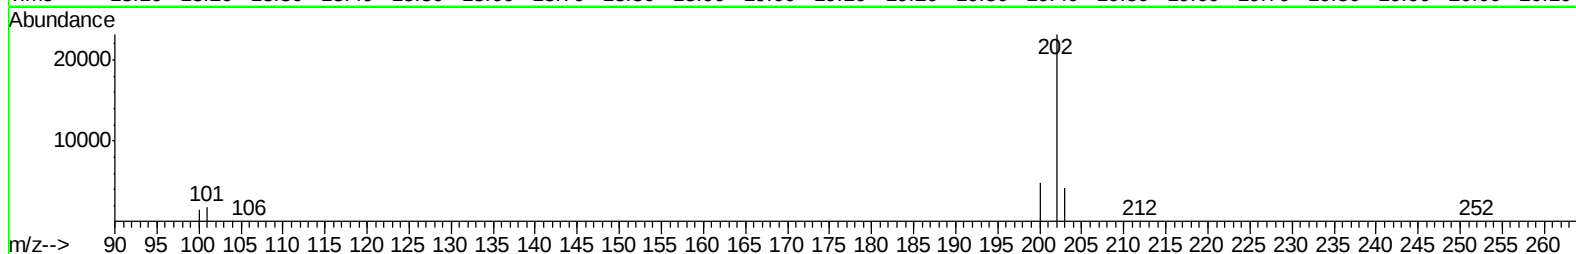


Data File : BM021828.D
Acq On : 05 Aug 2019 01:43
Operator : HP/JU
Sample : K3863-16
Misc :
ALS Vial : 71 Sample Multiplier: 1

Quant Time: Aug 05 08:43:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

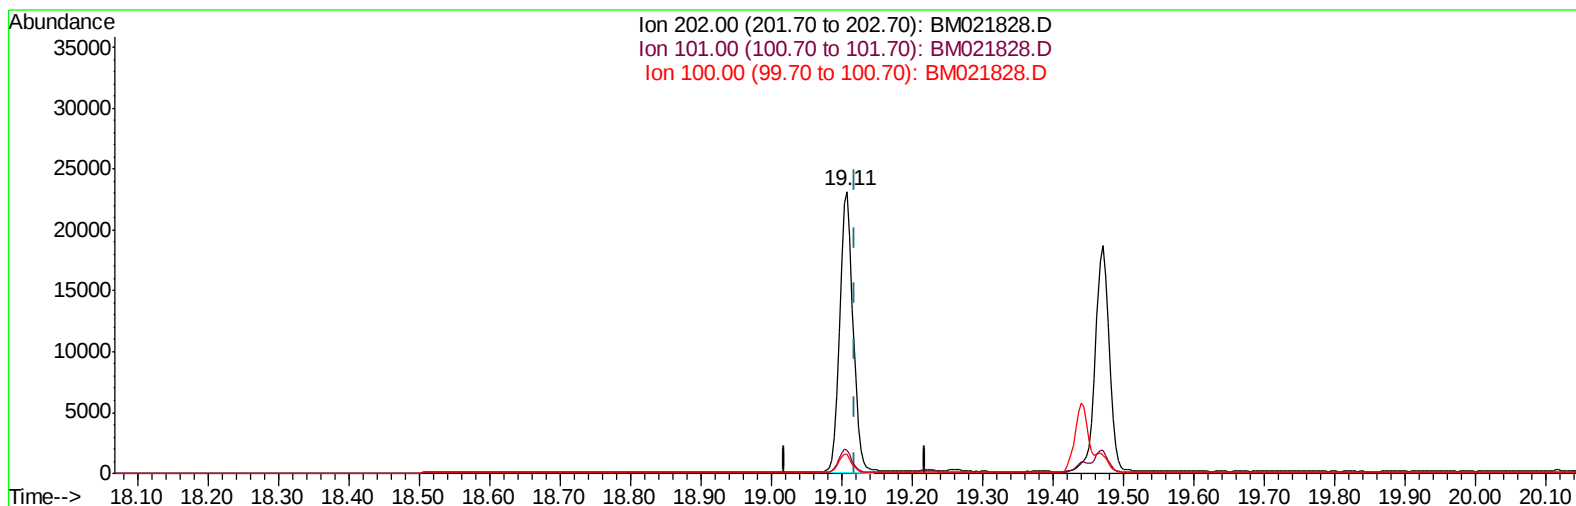

TIC: BM021828.D

(15) Fluoranthene (C)

19.108min (-0.011) 1.16ng/ul m

response 30545

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	8.17
100.00	8.10	6.66
0.00	0.00	0.00