
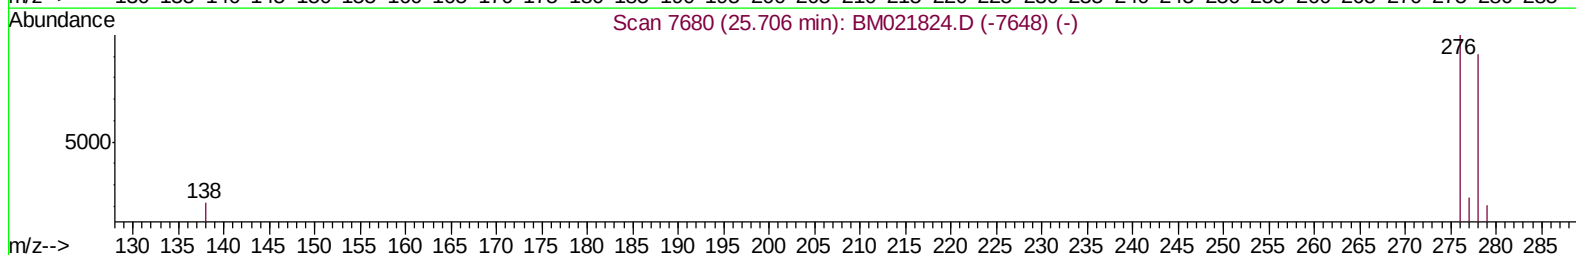
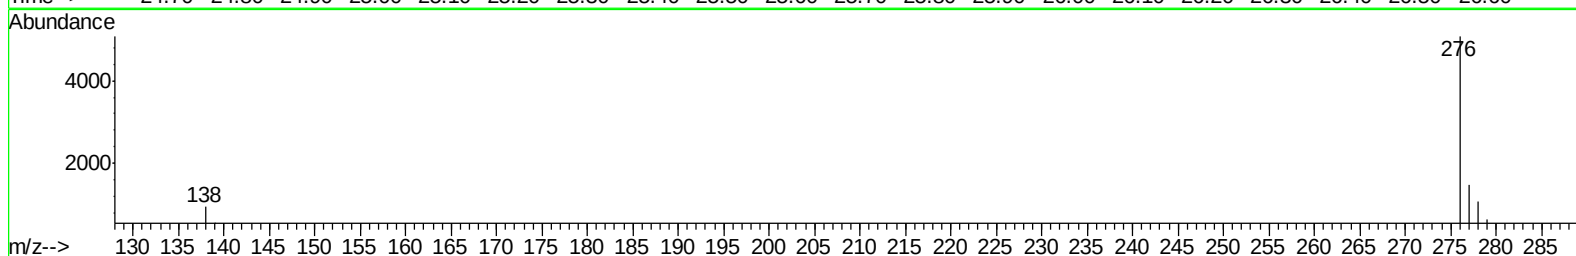


Data File : BM021828.D
Acq On : 05 Aug 2019 01:43
Operator : HP/JU
Sample : K3863-16
Misc :
ALS Vial : 71 Sample Multiplier: 1

Quant Time: Aug 05 08:45:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

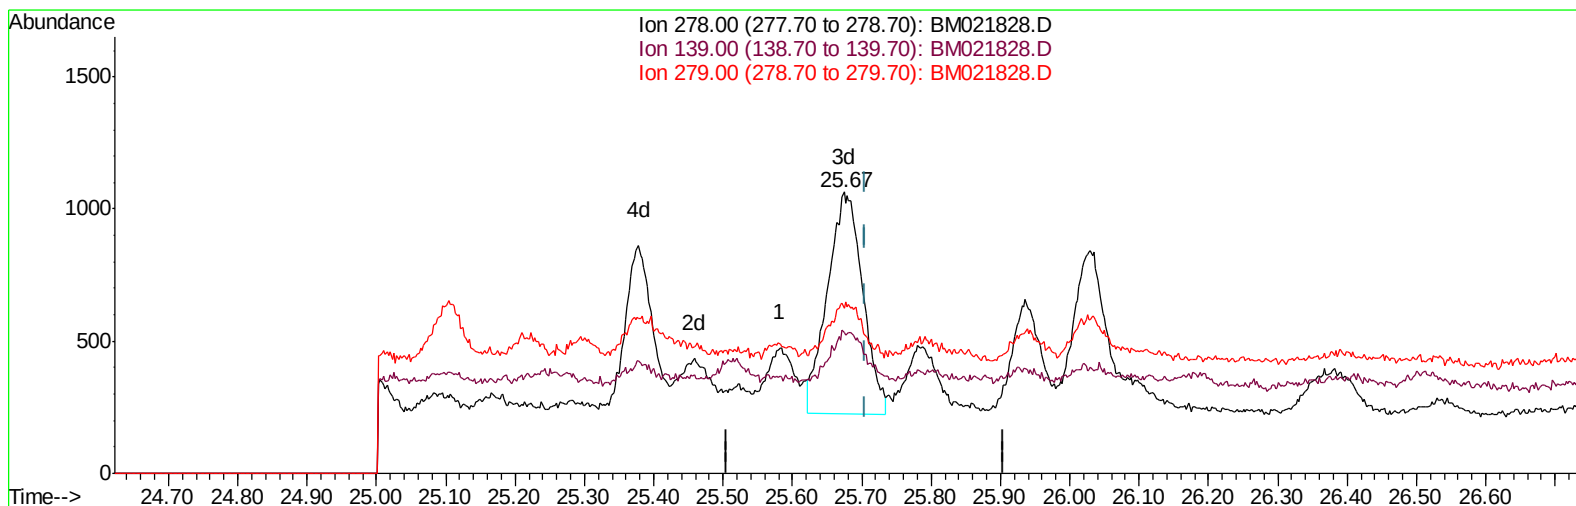

TIC: BM021828.D

(25) Dibenzo(a,h)anthracene

25.674min (-0.032) 0.12ng/ul m

response 2969

Ion	Exp%	Act%
278.00	100	100
139.00	17.70	50.23#
279.00	35.40	58.87#
0.00	0.00	0.00