
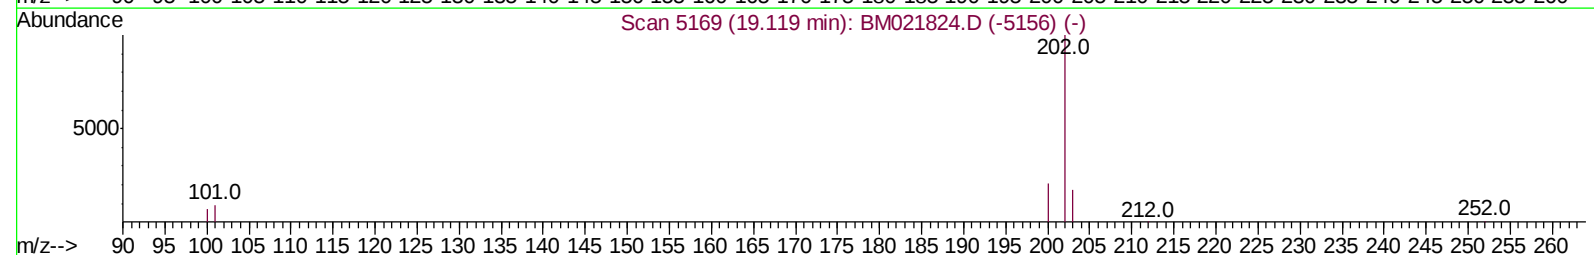
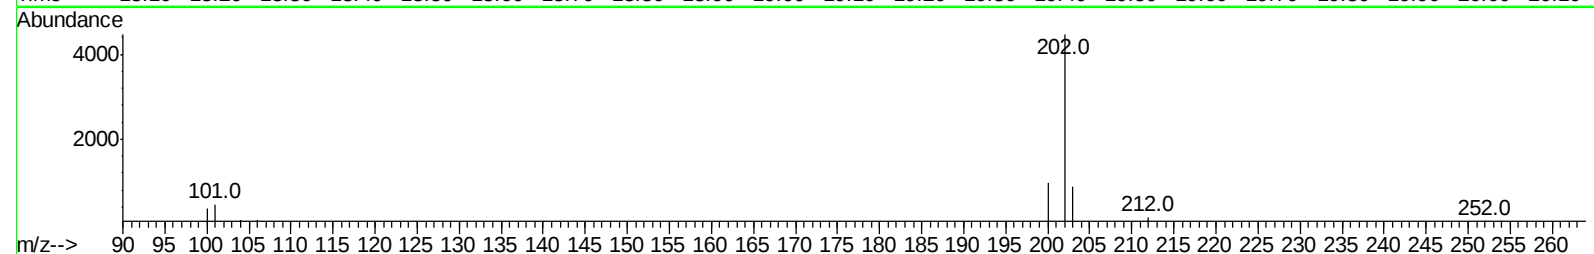


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\
Data File : BM021830.D
Acq On : 05 Aug 2019 02:56
Operator : HP/JU
Sample : K3863-03RE
Misc :
ALS Vial : 73 Sample Multiplier: 1

Quant Time: Aug 05 08:56:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 08:19:16 2019
Response via : Initial Calibration

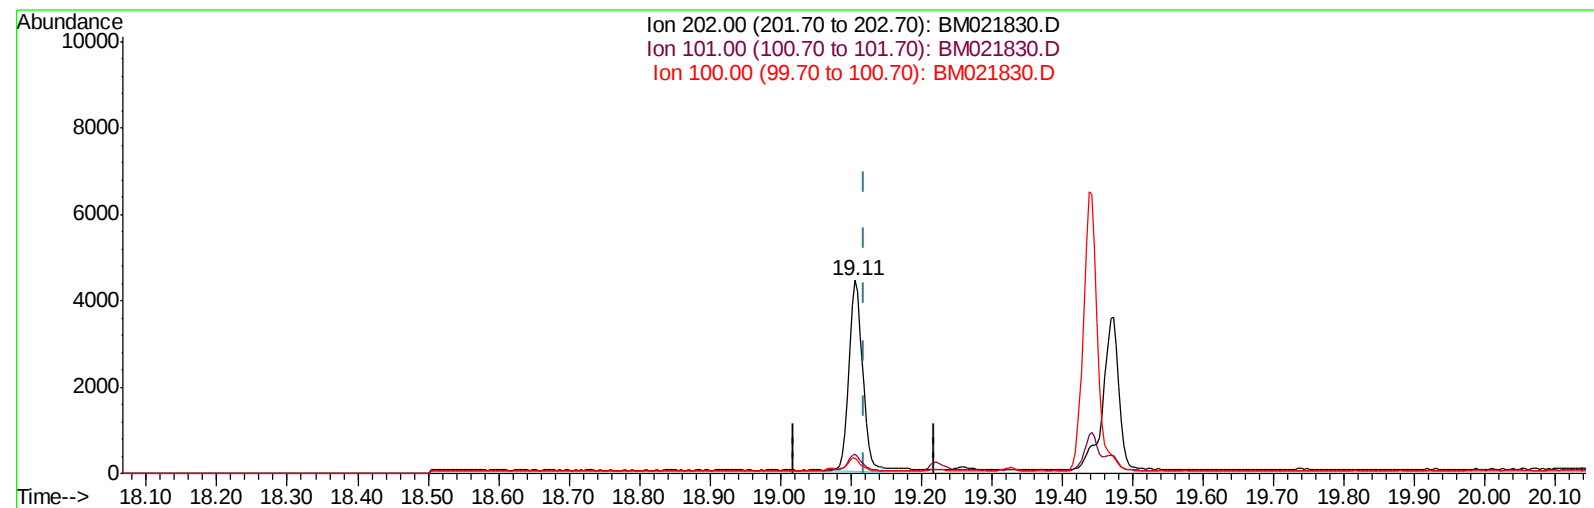

TIC: BM021830.D

(15) Fluoranthene (C)

19.106min (-0.013) 0.25ng/ul m

response 5978

Ion	Exp%	Act%
202.00	100	100
101.00	10.20	10.29
100.00	8.10	7.98
0.00	0.00	0.00