
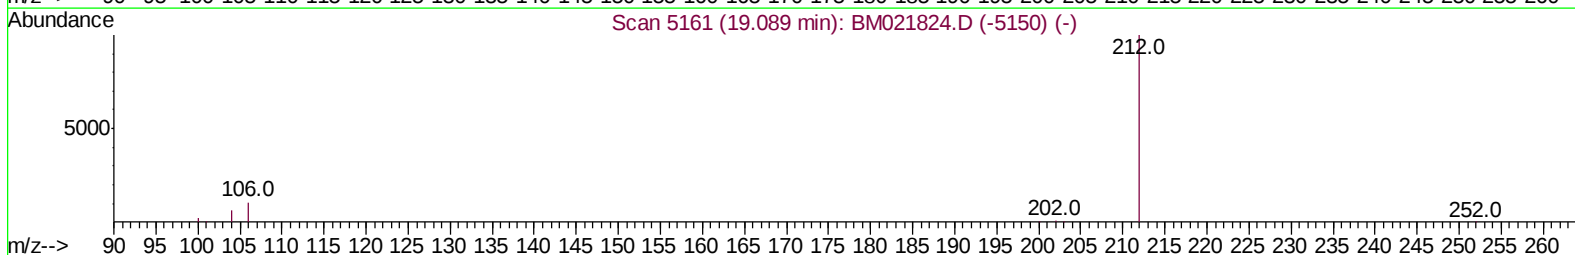
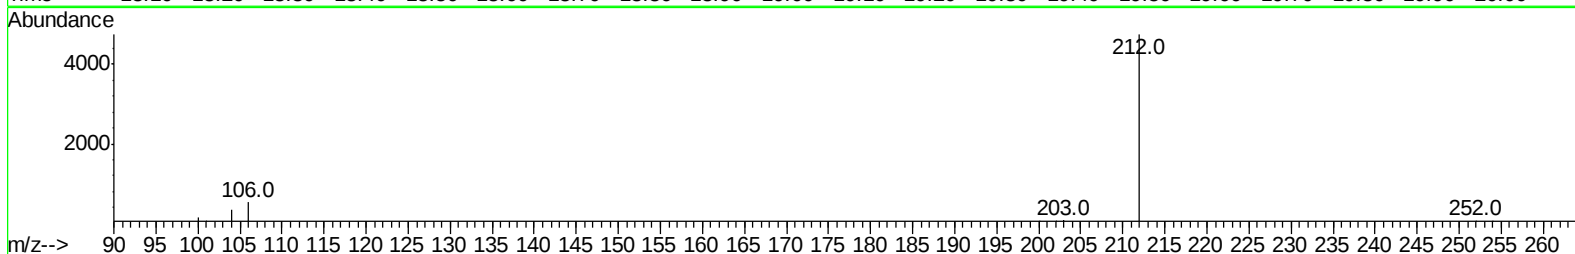


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM080319\  
Data File : BM021832.D  
Acq On : 05 Aug 2019 04:08  
Operator : HP/JU  
Sample : PB121644BL  
Misc :  
ALS Vial : 75 Sample Multiplier: 1

Quant Time: Aug 05 09:04:37 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

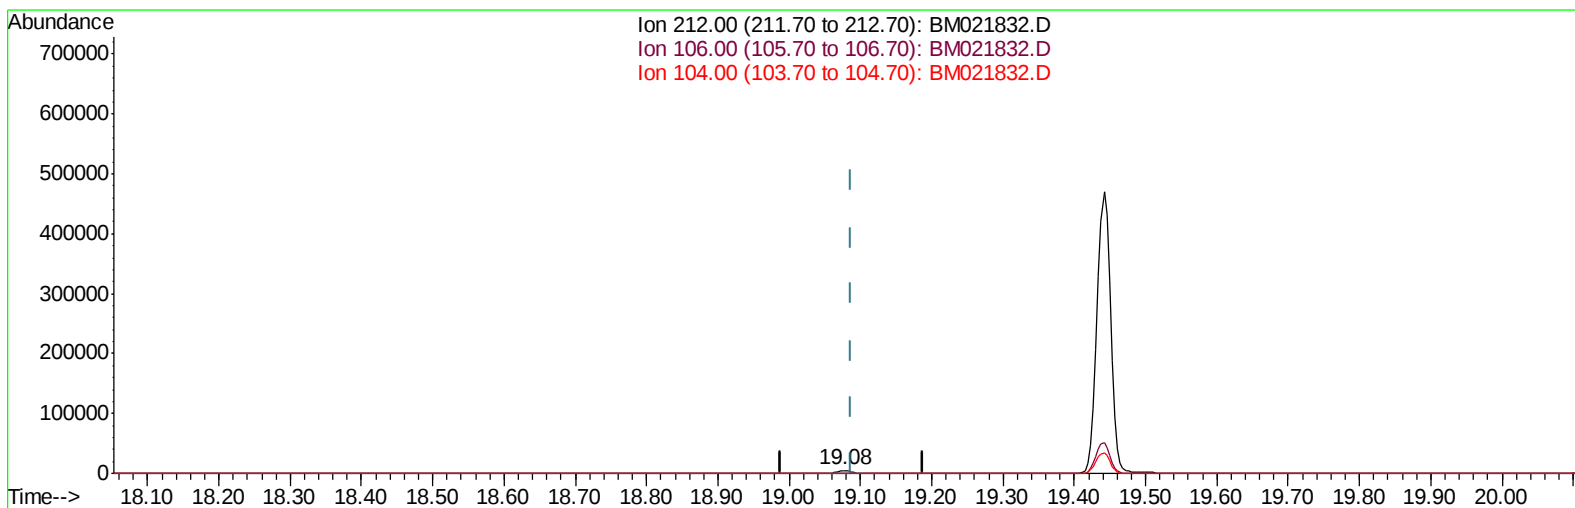

TIC: BM021832.D

(14) Fluoranthene-d10 (SURR)

19.076min (-0.013) 0.30ng/ul m

response 6495

| Ion    | Exp% | Act%  |
|--------|------|-------|
| 212.00 | 100  | 100   |
| 106.00 | 9.90 | 0.00# |
| 104.00 | 6.00 | 0.00# |
| 0.00   | 0.00 | 0.00  |