

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080319\
 Data File : BM021796.D
 Acq On : 04 Aug 2019 05:05
 Operator : HP/JU
 Sample : K3863-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 04 08:57:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 04 04:24:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1087	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	4225	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.29	164	2486	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.14	188	371939	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.31	264	522777	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	1729	0.25	ng/ul	-0.03
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.01	152	304	0.026	ng/ul#	Ovalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080319\
Data File : BM021796.D
Acq On : 04 Aug 2019 05:05
Operator : HP/JU
Sample : K3863-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 04 08:57:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

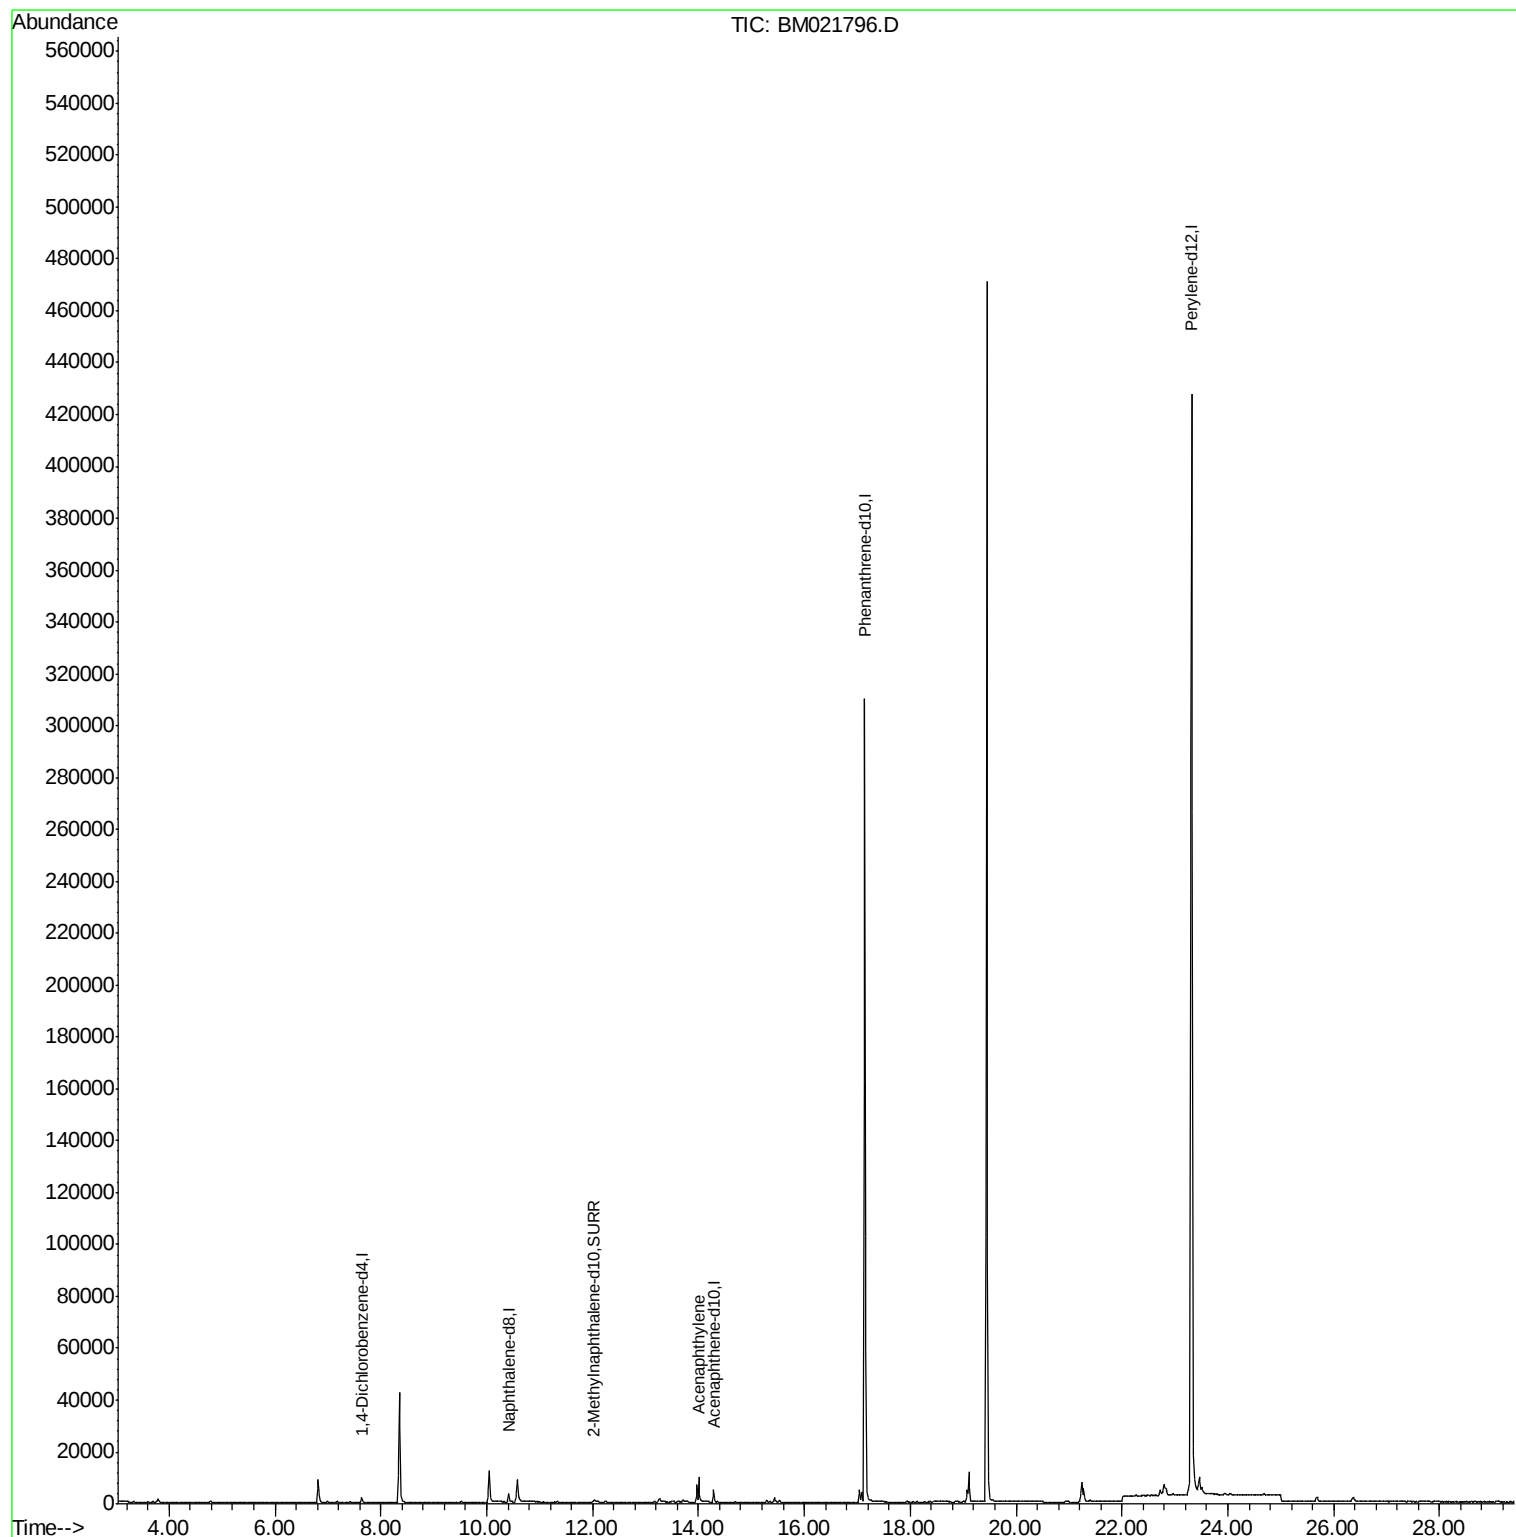

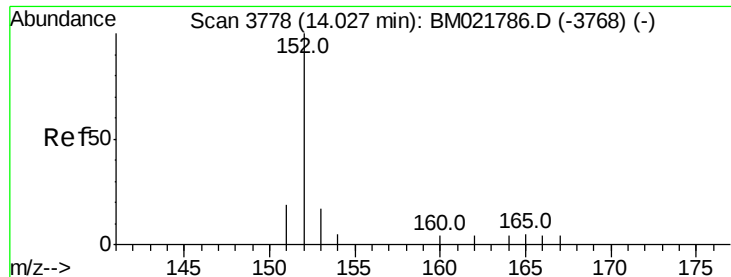

#7

Acenaphthylene

Concen: 0.026 ng/ul

RT: 14.01 min Scan# 3773

Delta R.T. -0.02 min

Lab File: BM021796.D

Acq: 04 Aug 2019 05:05

Instrument :

BNA_M

ClientSampleId :

Tot Ion:	152	Resp:	304
Ion	Ratio	Lower	Upper
152	100		
151	40.6	18.3	27.5#
153	37.2	12.8	19.2#

