

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080319\
 Data File : BM021801.D
 Acq On : 04 Aug 2019 08:06
 Operator : HP/JU
 Sample : K3863-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Aug 04 08:57:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Aug 04 04:24:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1078	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.41	136	4223	0.40	ng/ul	-0.03
6) Acenaphthene-d10	14.29	164	2394	0.40	ng/ul	-0.02
10) Phenanthrene-d10	17.14	188	336931	0.40	ng/ul	0.07
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.26
20) Perylene-d12	23.31	264	434718	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	1487	0.21	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.29	166	568	0.056	ng/ul#	Ovalue 21




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM080319\
Data File : BM021801.D
Acq On : 04 Aug 2019 08:06
Operator : HP/JU
Sample : K3863-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Aug 04 08:57:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Aug 04 04:24:24 2019
Response via : Initial Calibration

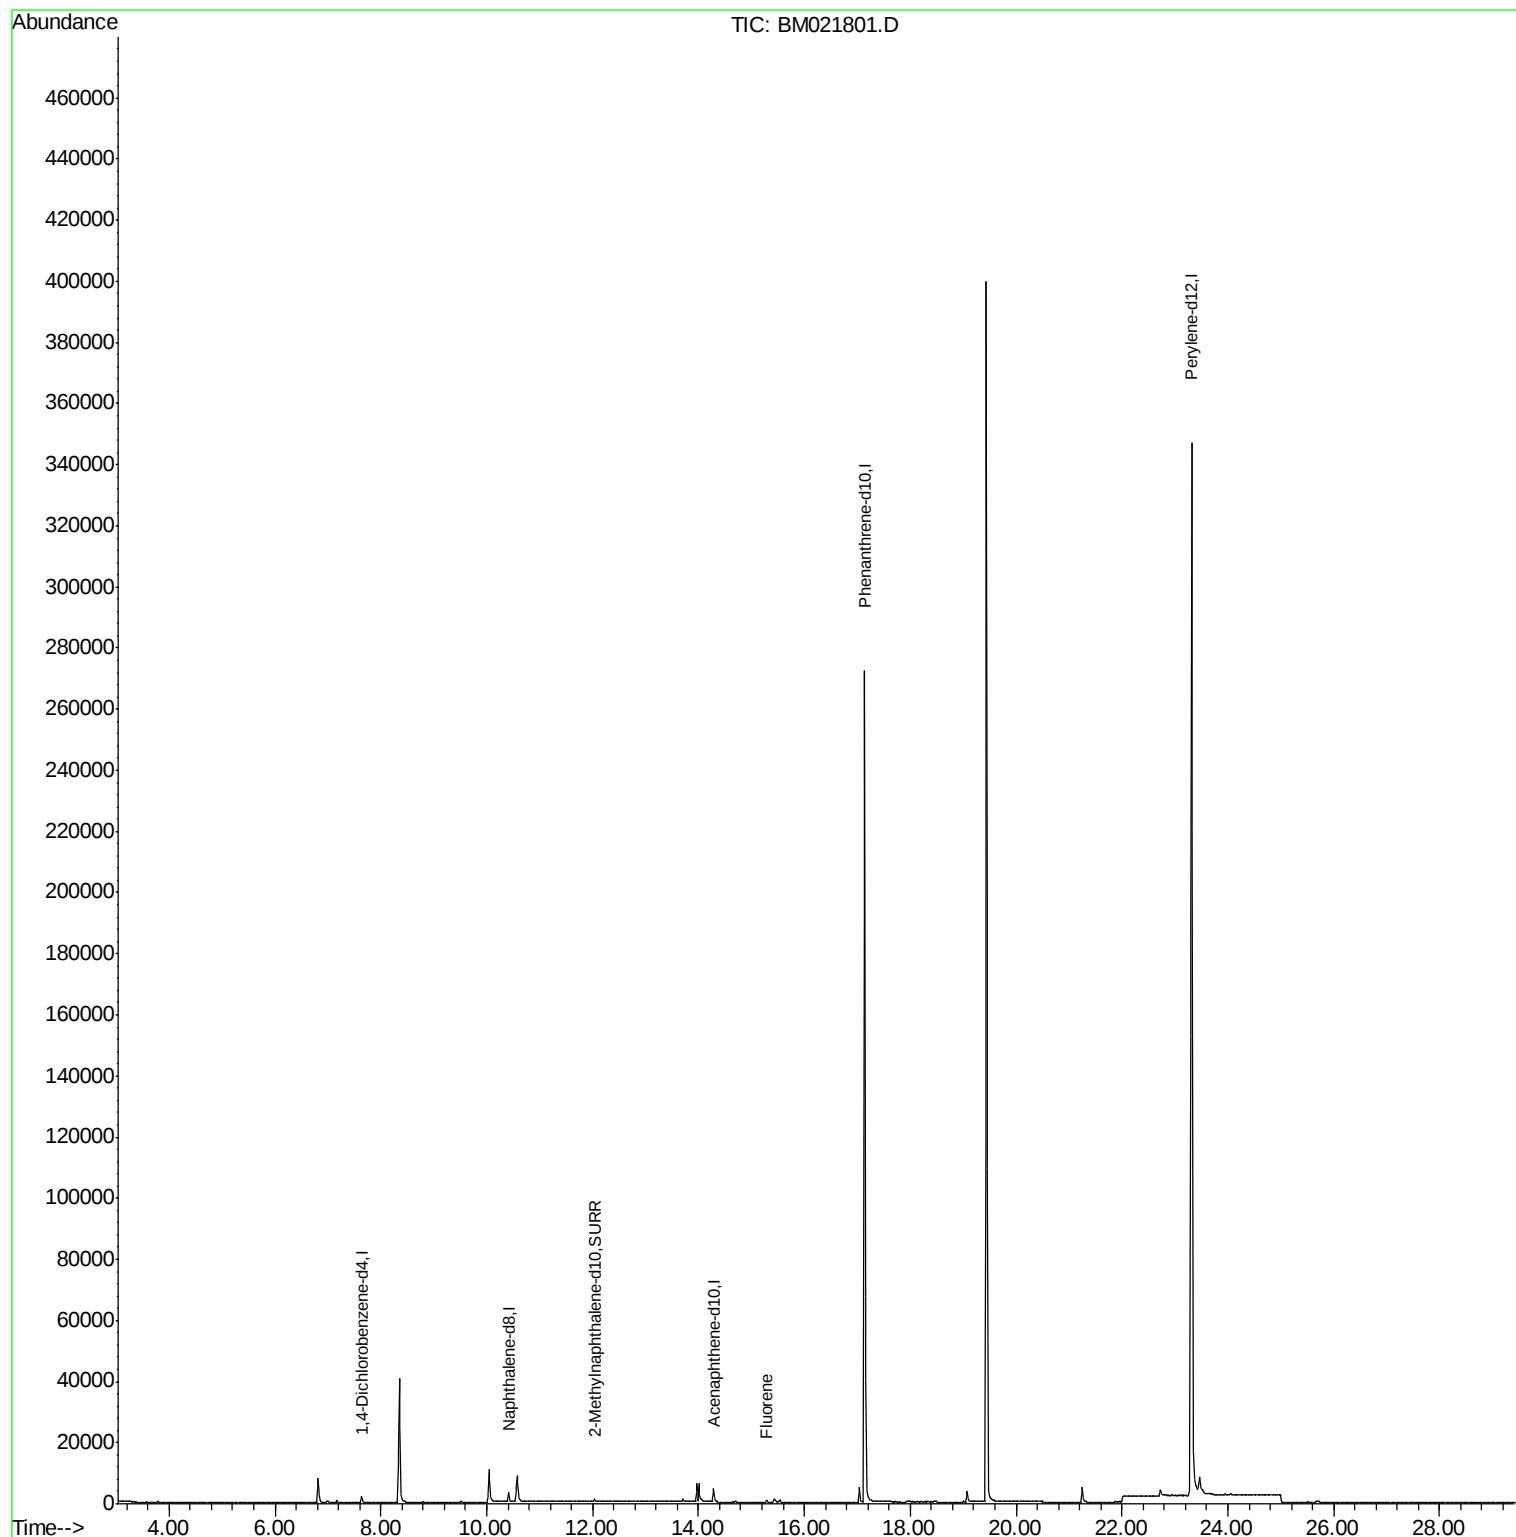

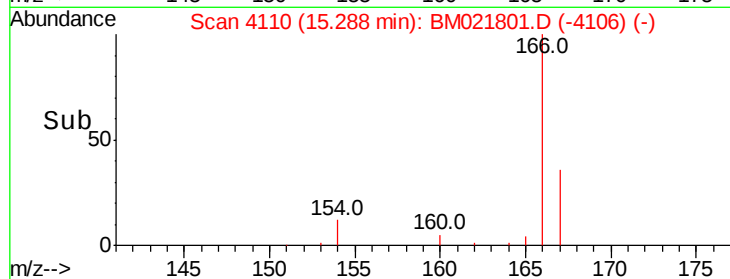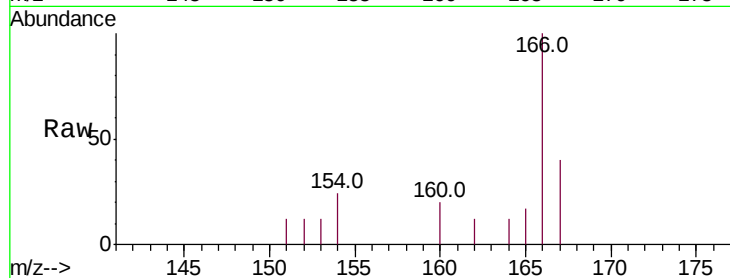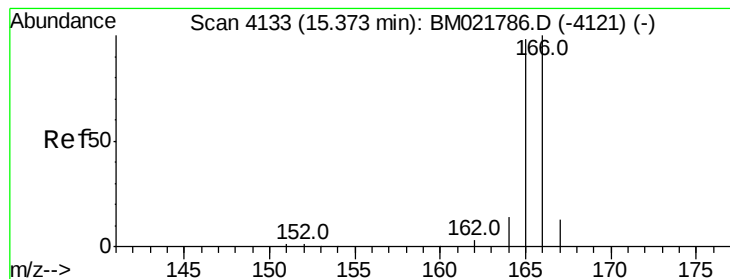

#9

Fluorene

Concen: 0.056 ng/ul

RT: 15.29 min Scan# 4110

Delta R.T. -0.09 min

Lab File: BM021801.D

Acq: 04 Aug 2019 08:06

Instrument :

BNA_M

ClientSampleId :

Tot Ion:166 Resp: 568

Ion Ratio Lower Upper

166 100

165 16.8 81.4 122.0#

167 39.5 13.7 20.5#

