

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Not Reviewed)

Data File : BM021805.D
Acq On : 04 Aug 2019 10:32
Operator : HP/JU
Sample : K3863-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52J0

Quant Time: Aug 05 05:29:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	1044	0.40	ng/ul	0.00
2) Naphthalene-d8	10.42	136	4105	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.29	164	2346	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	238193	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.32	264	571378	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.04	152	1109	0.16	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.29	166	445	0.045	ng/ul#	Qvalue 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021805.D
Acq On : 04 Aug 2019 10:32
Operator : HP/JU
Sample : K3863-09
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52J0

Quant Time: Aug 05 05:29:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 05:26:43 2019
Response via : Initial Calibration

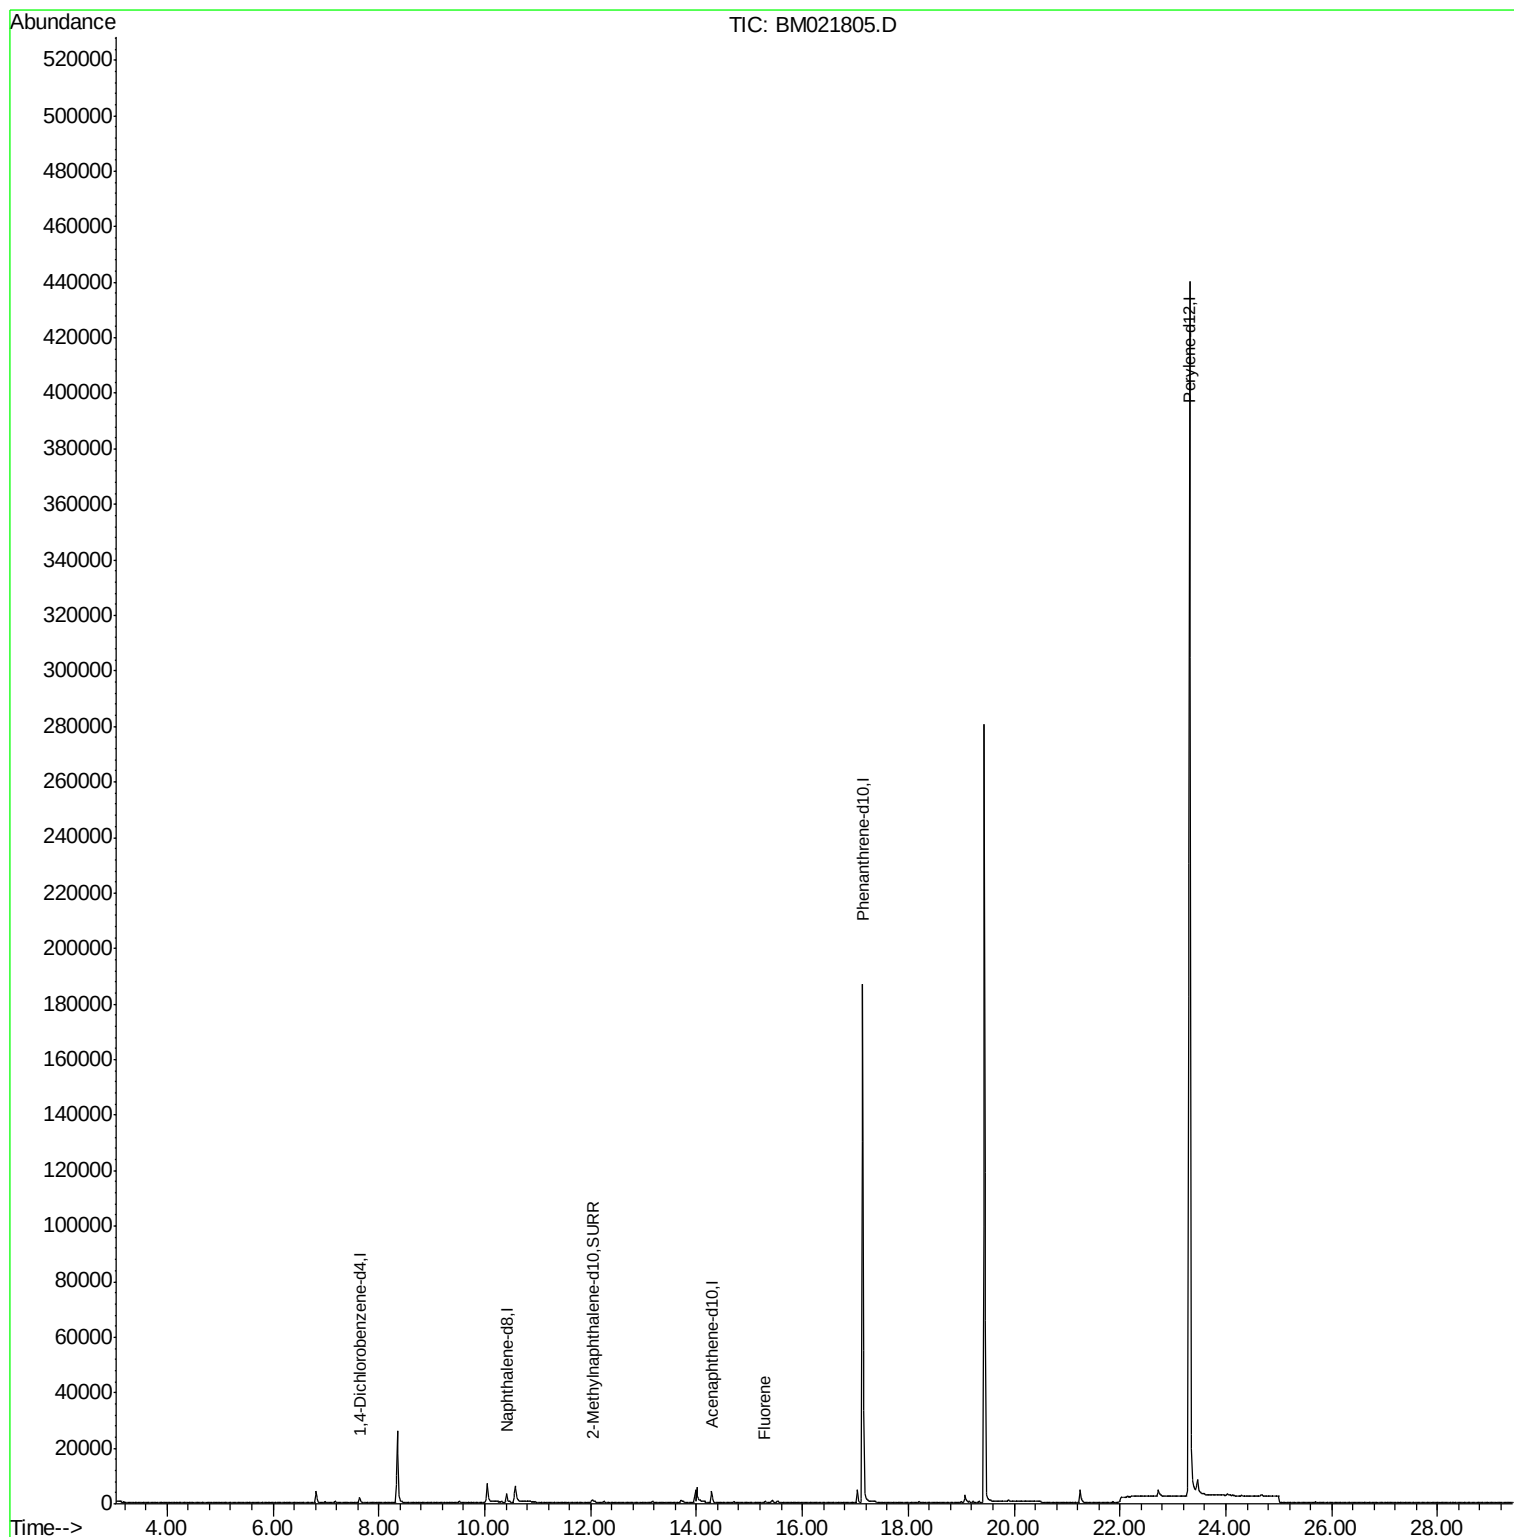

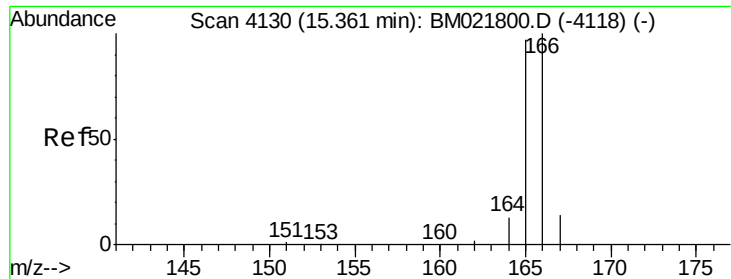

#9

Fluorene

Concen: 0.045 ng/ul

RT: 15.29 min Scan# 4110

Delta R.T. -0.07 min

Lab File: BM021805.D


Acq: 04 Aug 2019 10:32

Instrument :

BNA_M

ClientSampleId :

A52J0

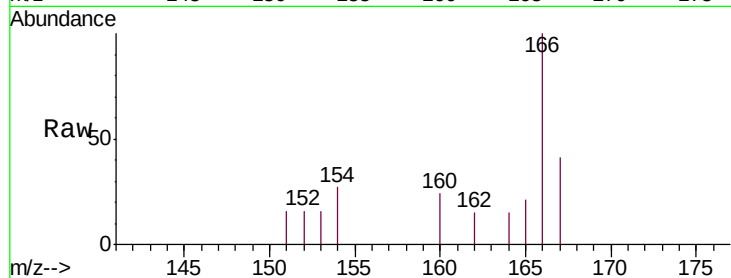


Tgt Ion:166 Resp: 445

Ion Ratio Lower Upper

166 100

165 20.9 81.4 122.0#

167 40.6 13.7 20.5#

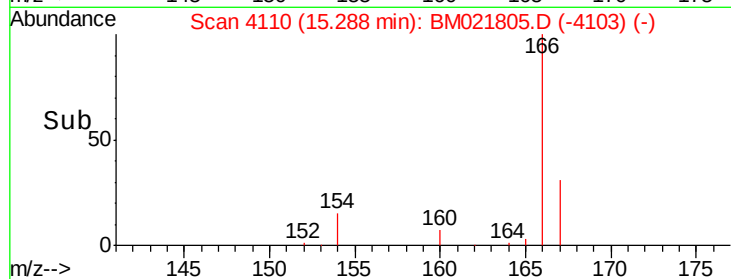

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

