

Data File : BM021823.D
Acq On : 04 Aug 2019 21:28
Operator : HP/JU
Sample : K4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DB8K9

Quant Time: Aug 05 07:01:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 06:57:04 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	938	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3823	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.29	164	2204	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	442837	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.25
20) Perylene-d12	23.31	264	613938	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	1833	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.28	166	755	0.081	ng/ul#	Qvalue 19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021823.D
Acq On : 04 Aug 2019 21:28
Operator : HP/JU
Sample : K4128-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DB8K9

Quant Time: Aug 05 07:01:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 05 06:57:04 2019
Response via : Initial Calibration

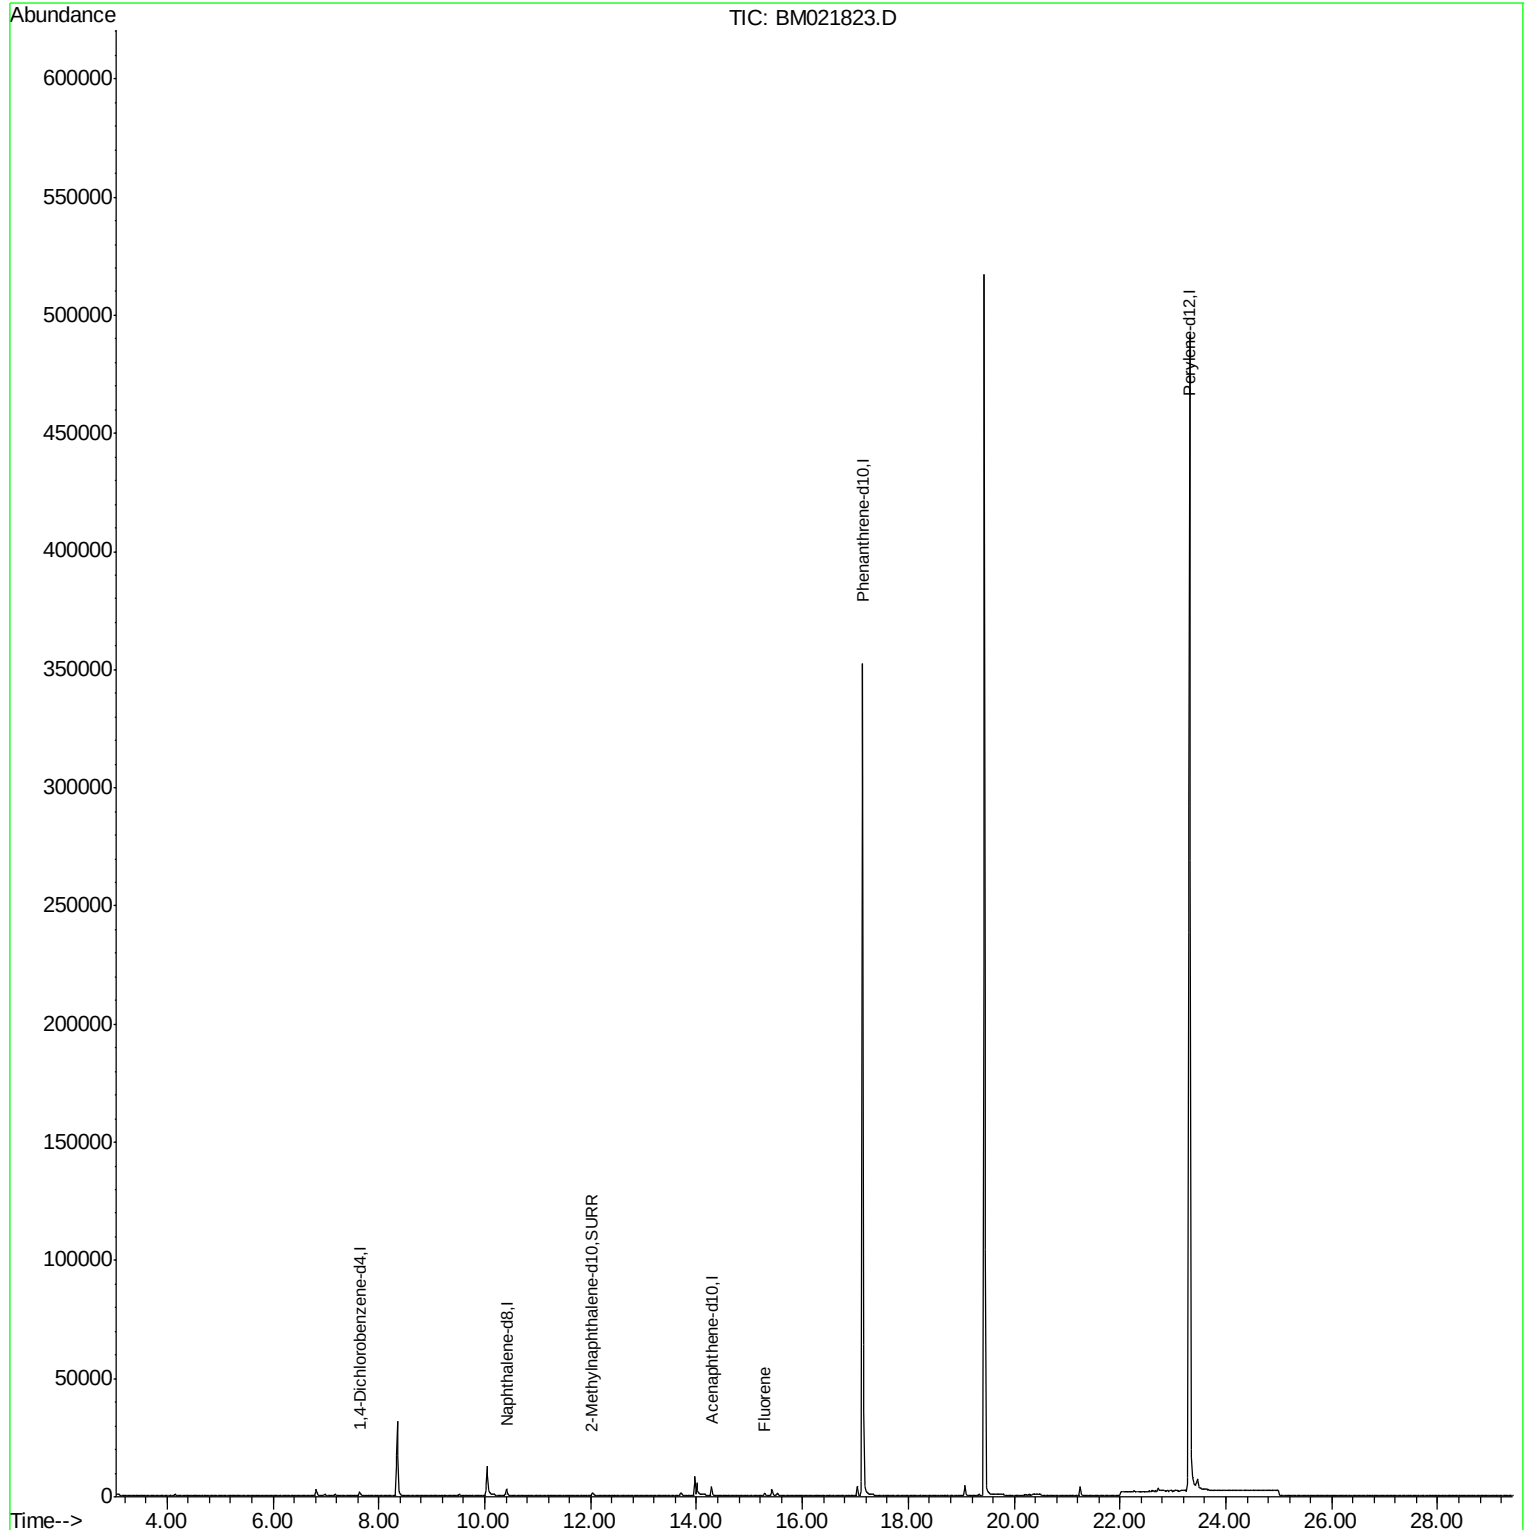

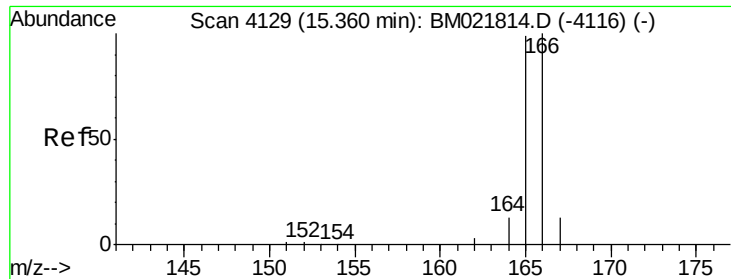

#9

Fluorene

Concen: 0.081 ng/ul

RT: 15.28 min Scan# 4109

Delta R.T. -0.08 min

Lab File: BM021823.D


Acq: 04 Aug 2019 21:28

Instrument :

BNA_M

ClientSampleId :

DB8K9

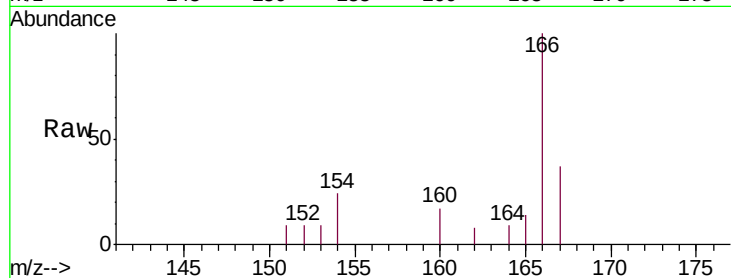


Tgt Ion:166 Resp: 755

Ion Ratio Lower Upper

166 100

165 13.5 81.4 122.0#

167 36.9 13.7 20.5#

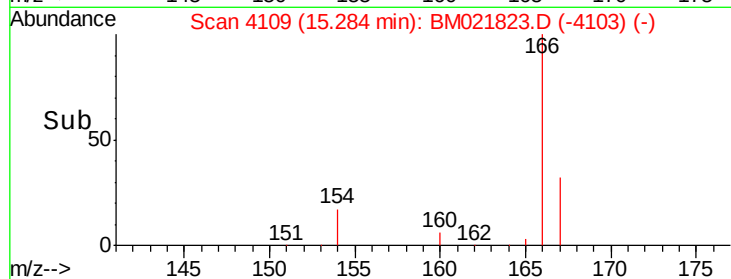

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

