

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM080319\  
Quantitation Report (Not Reviewed)

Data File : BM021832.D  
Acq On : 05 Aug 2019 04:08  
Operator : HP/JU  
Sample : PB121644BL  
Misc :  
ALS Vial : 75 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK44

Quant Time: Aug 05 08:24:42 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc  | Units  | Dev(Min)  |
|-----------------------------|-------|------|----------|-------|--------|-----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.64  | 152  | 1082     | 0.40  | ng/ul  | 0.00      |
| 2) Naphthalene-d8           | 10.41 | 136  | 4525     | 0.40  | ng/ul  | -0.02     |
| 6) Acenaphthene-d10         | 14.29 | 164  | 2682     | 0.40  | ng/ul  | 0.00      |
| 10) Phenanthrene-d10        | 17.14 | 188  | 509199   | 0.40  | ng/ul  | 0.08      |
| 16) Chrysene-d12            | 0.00  | 240  | 0        | 0.00  | ng/ul  | -21.25    |
| 20) Perylene-d12            | 23.31 | 264  | 626636   | 0.40  | ng/ul  | -0.16     |
| System Monitoring Compounds |       |      |          |       |        |           |
| 4) 2-Methylnaphthalene-d10  | 12.03 | 152  | 2285     | 0.31  | ng/ul  | -0.01     |
| 14) Fluoranthene-d10        | 0.00  | 212  | 0        | 0.00  | ng/ul  |           |
| Target Compounds            |       |      |          |       |        |           |
| 9) Fluorene                 | 15.28 | 166  | 864      | 0.076 | ng/ul# | Qvalue 18 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021832.D  
Acq On : 05 Aug 2019 04:08  
Operator : HP/JU  
Sample : PB121644BL  
Misc :  
ALS Vial : 75 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK44

Quant Time: Aug 05 08:24:42 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

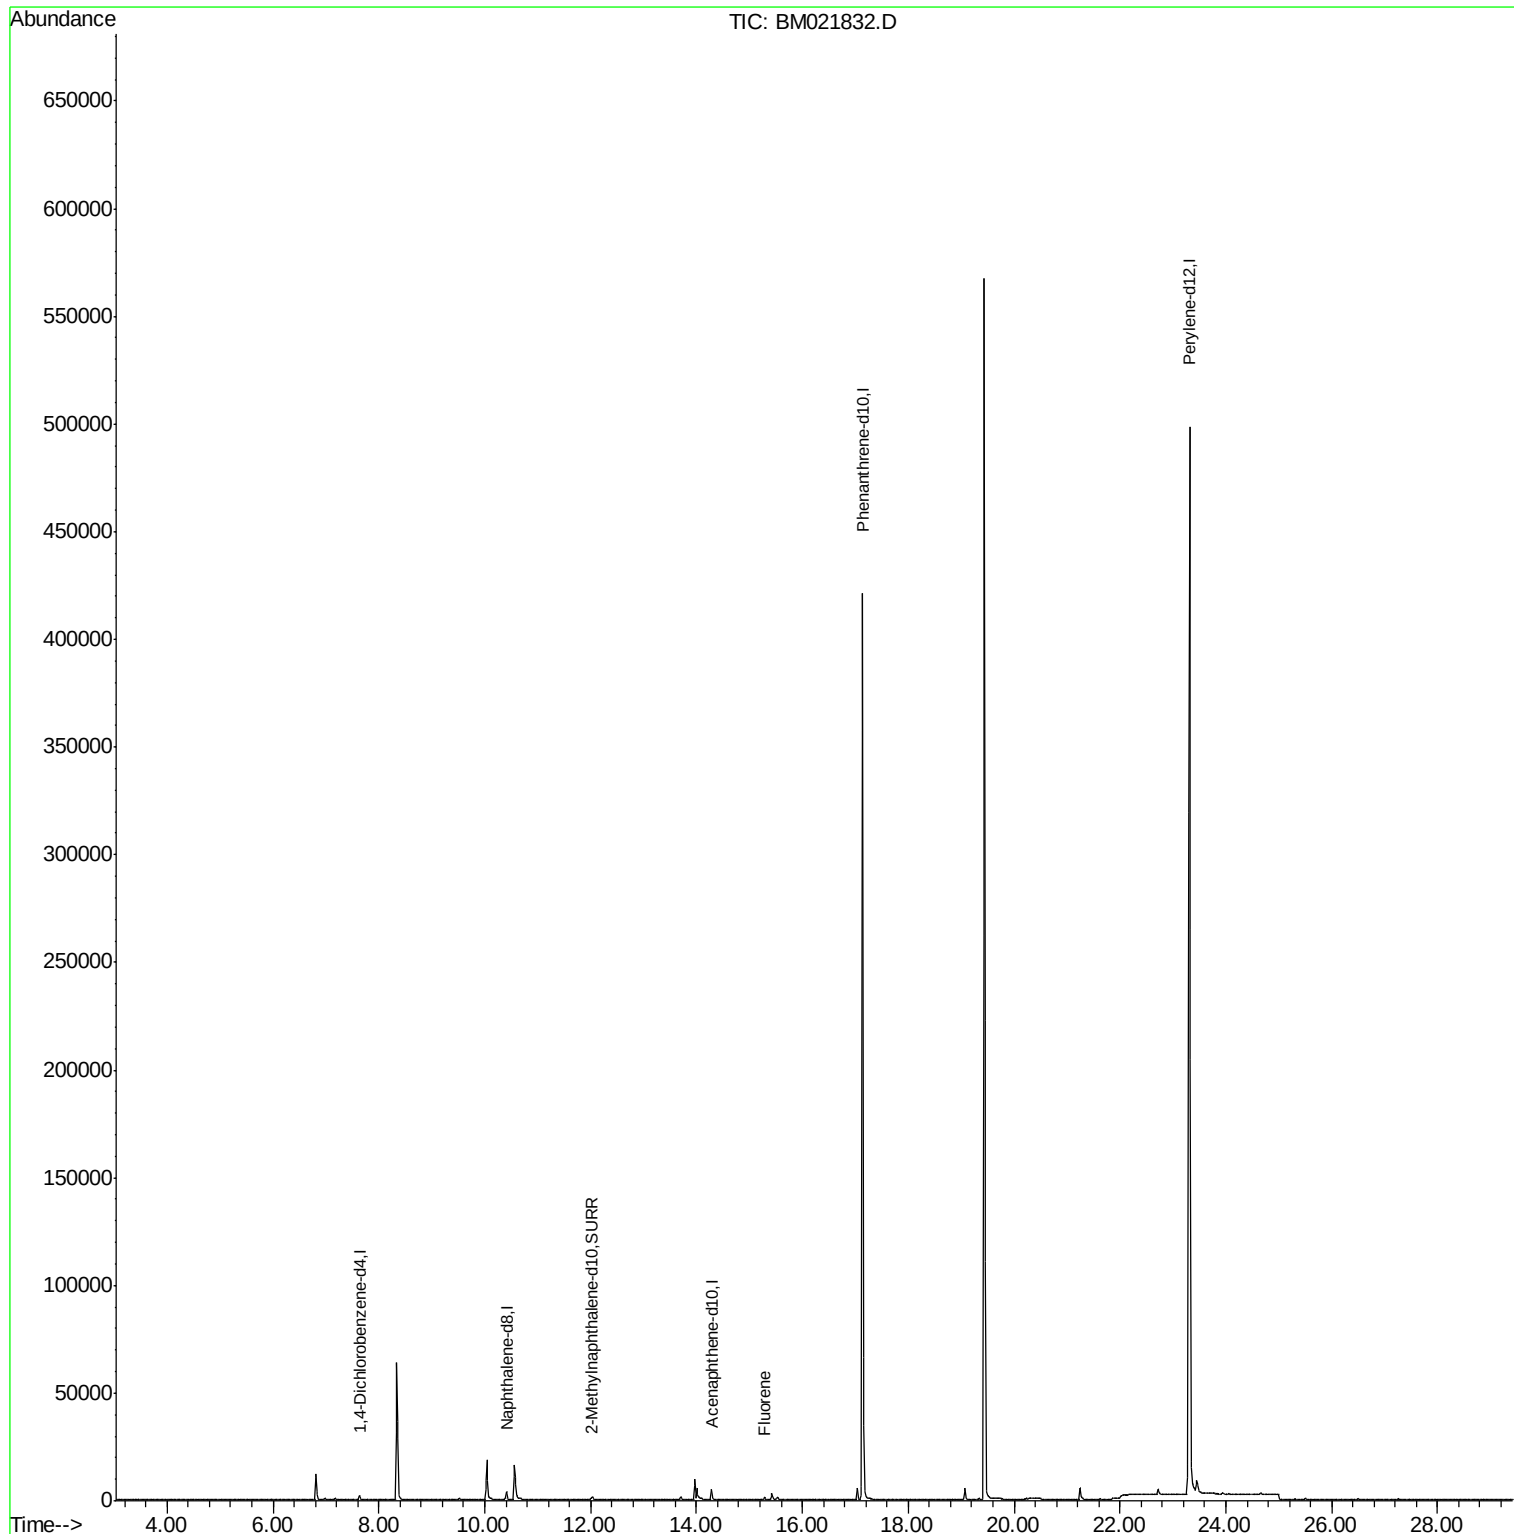

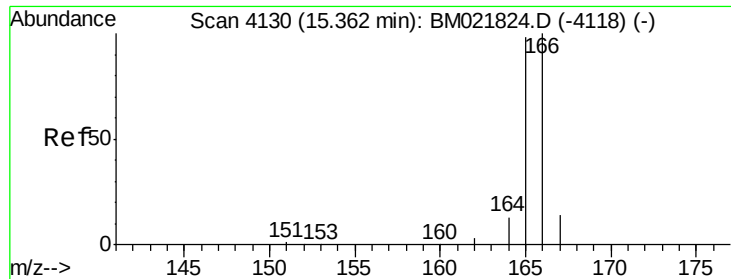

#9

Fluorene

Concen: 0.076 ng/ul

RT: 15.28 min Scan# 4109

Delta R.T. -0.08 min

Lab File: BM021832.D

Acq: 05 Aug 2019 04:08

Instrument :

BNA\_M

ClientSampleId :

SBLK44

Tgt Ion:166 Resp: 864

Ion Ratio Lower Upper

166 100

165 13.0 81.4 122.0#

167 37.7 13.7 20.5#

