

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM080319\  
Quantitation Report (Not Reviewed)

Data File : BM021833.D  
Acq On : 05 Aug 2019 04:45  
Operator : HP/JU  
Sample : PB121548BL  
Misc :  
ALS Vial : 76 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK48

Quant Time: Aug 05 08:24:49 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration


| Internal Standards          | R.T.  | QIon | Response | Conc  | Units  | Dev(Min) |
|-----------------------------|-------|------|----------|-------|--------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 7.64  | 152  | 1122     | 0.40  | ng/ul  | 0.00     |
| 2) Naphthalene-d8           | 10.41 | 136  | 4511     | 0.40  | ng/ul  | -0.02    |
| 6) Acenaphthene-d10         | 14.28 | 164  | 2560     | 0.40  | ng/ul  | -0.01    |
| 10) Phenanthrene-d10        | 17.14 | 188  | 486952   | 0.40  | ng/ul  | 0.08     |
| 16) Chrysene-d12            | 0.00  | 240  | 0        | 0.00  | ng/ul  | -21.25   |
| 20) Perylene-d12            | 23.31 | 264  | 602334   | 0.40  | ng/ul  | -0.16    |
| System Monitoring Compounds |       |      |          |       |        |          |
| 4) 2-Methylnaphthalene-d10  | 12.03 | 152  | 2308     | 0.31  | ng/ul  | -0.01    |
| 14) Fluoranthene-d10        | 0.00  | 212  | 0        | 0.00  | ng/ul  |          |
| Target Compounds            |       |      |          |       |        |          |
| 9) Fluorene                 | 15.29 | 166  | 874      | 0.081 | ng/ul# | 18       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021833.D  
Acq On : 05 Aug 2019 04:45  
Operator : HP/JU  
Sample : PB121548BL  
Misc :  
ALS Vial : 76 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
SBLK48

Quant Time: Aug 05 08:24:49 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-SIM-BM080319.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 05 08:19:16 2019  
Response via : Initial Calibration

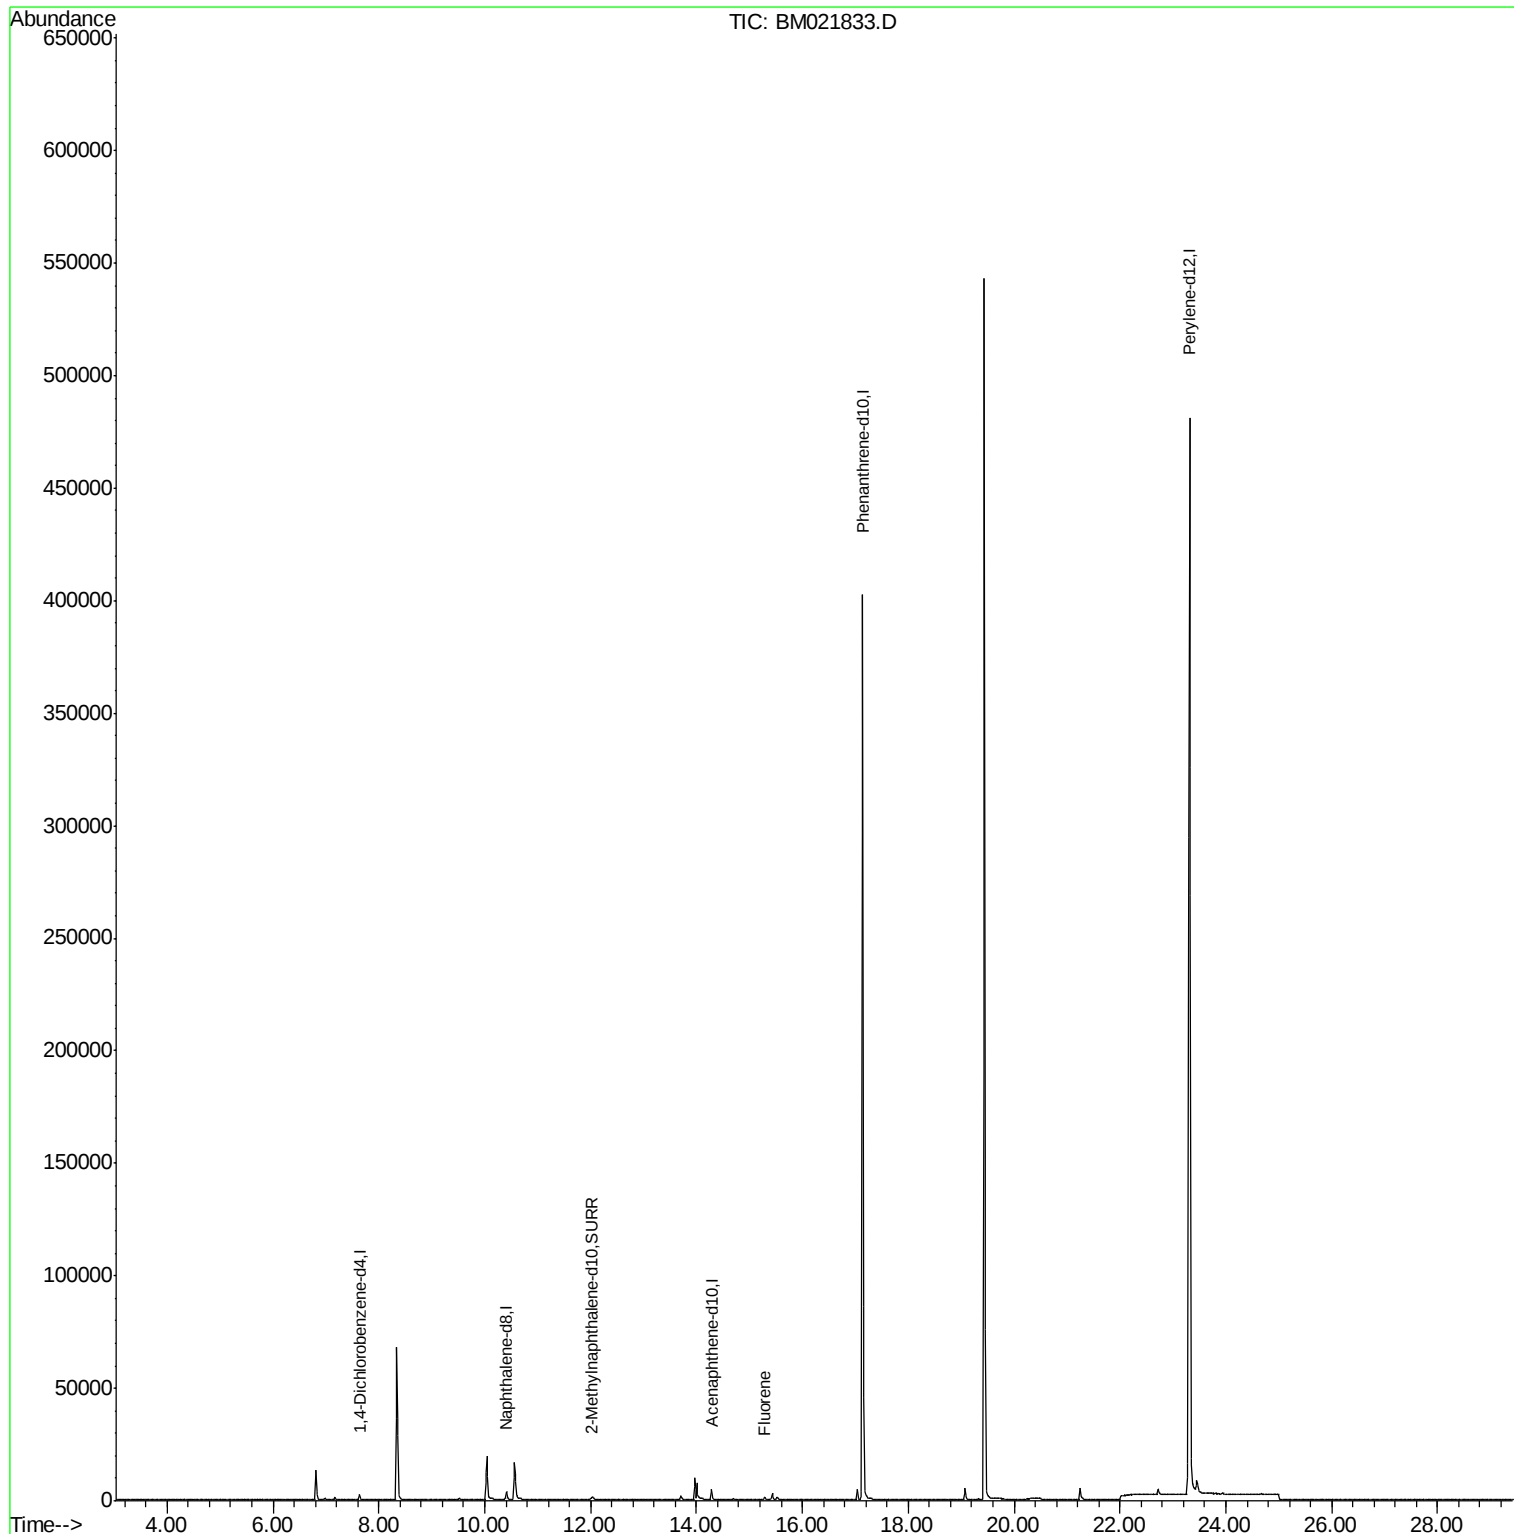

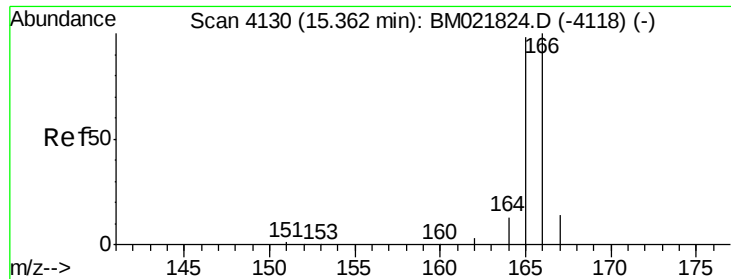

#9

Fluorene

Concen: 0.081 ng/ul

RT: 15.29 min Scan# 4110

Delta R.T. -0.08 min

Lab File: BM021833.D

Acq: 05 Aug 2019 04:45

Instrument :

BNA\_M

ClientSampleId :

SBLK48

Tgt Ion:166 Resp: 874

Ion Ratio Lower Upper

166 100

165 13.1 81.4 122.0#

167 37.5 13.7 20.5#

