

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Not Reviewed)

Data File : BM021849.D
Acq On : 05 Aug 2019 19:17
Operator : HP/JU
Sample : K3823-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52N8

Quant Time: Aug 06 01:32:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	812	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3440	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.28	164	2008	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	277075	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.31	264	364867	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	1291	0.23	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
7) Acenaphthylene	14.00	152	206	0.022	ng/ul#	Qvalue 53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021849.D
Acq On : 05 Aug 2019 19:17
Operator : HP/JU
Sample : K3823-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52N8

Quant Time: Aug 06 01:32:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

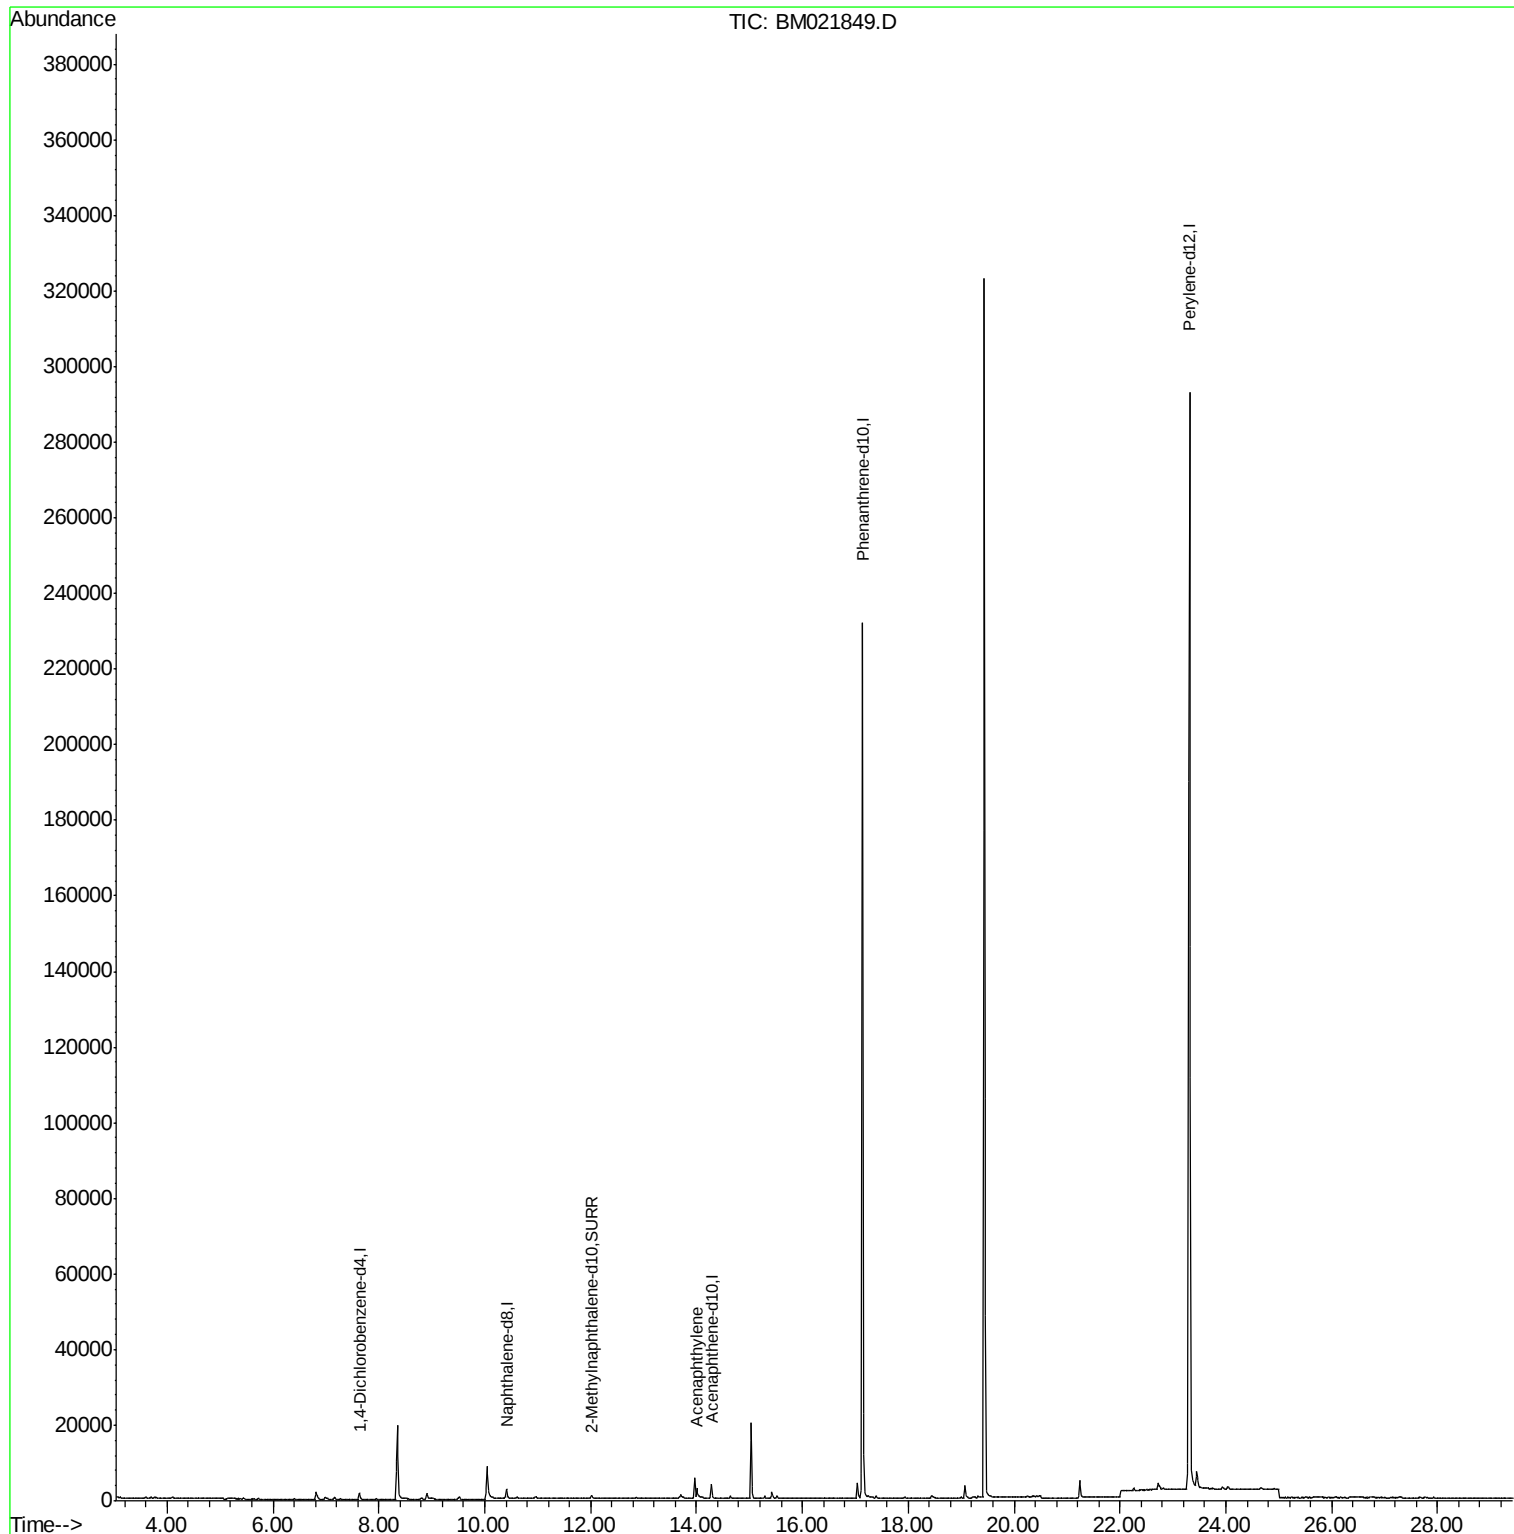

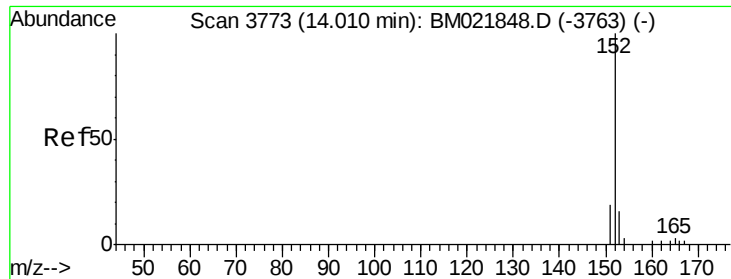

#7

Acenaphthylene

Concen: 0.022 ng/ul

RT: 14.00 min Scan# 3771

Delta R.T. -0.01 min

Lab File: BM021849.D

Acq: 05 Aug 2019 19:17

Instrument :

BNA_M

ClientSampleId :

A52N8

Tgt Ion:152 Resp: 206

Ion Ratio Lower Upper

152 100

151 49.0 18.3 27.5#

153 0.0 12.8 19.2#

