

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM080319\
Quantitation Report (Not Reviewed)

Data File : BM021851.D
Acq On : 05 Aug 2019 20:30
Operator : HP/JU
Sample : K3823-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52N6

Quant Time: Aug 06 01:32:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	842	0.40	ng/ul	0.00
2) Naphthalene-d8	10.41	136	3526	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.28	164	2061	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.14	188	403283	0.40	ng/ul	0.09
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.31	264	503674	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	1736	0.30	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.46	128	235	0.024	ng/ul#	Qvalue 51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM021851.D
Acq On : 05 Aug 2019 20:30
Operator : HP/JU
Sample : K3823-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A52N6

Quant Time: Aug 06 01:32:12 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM080319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 06 01:29:26 2019
Response via : Initial Calibration

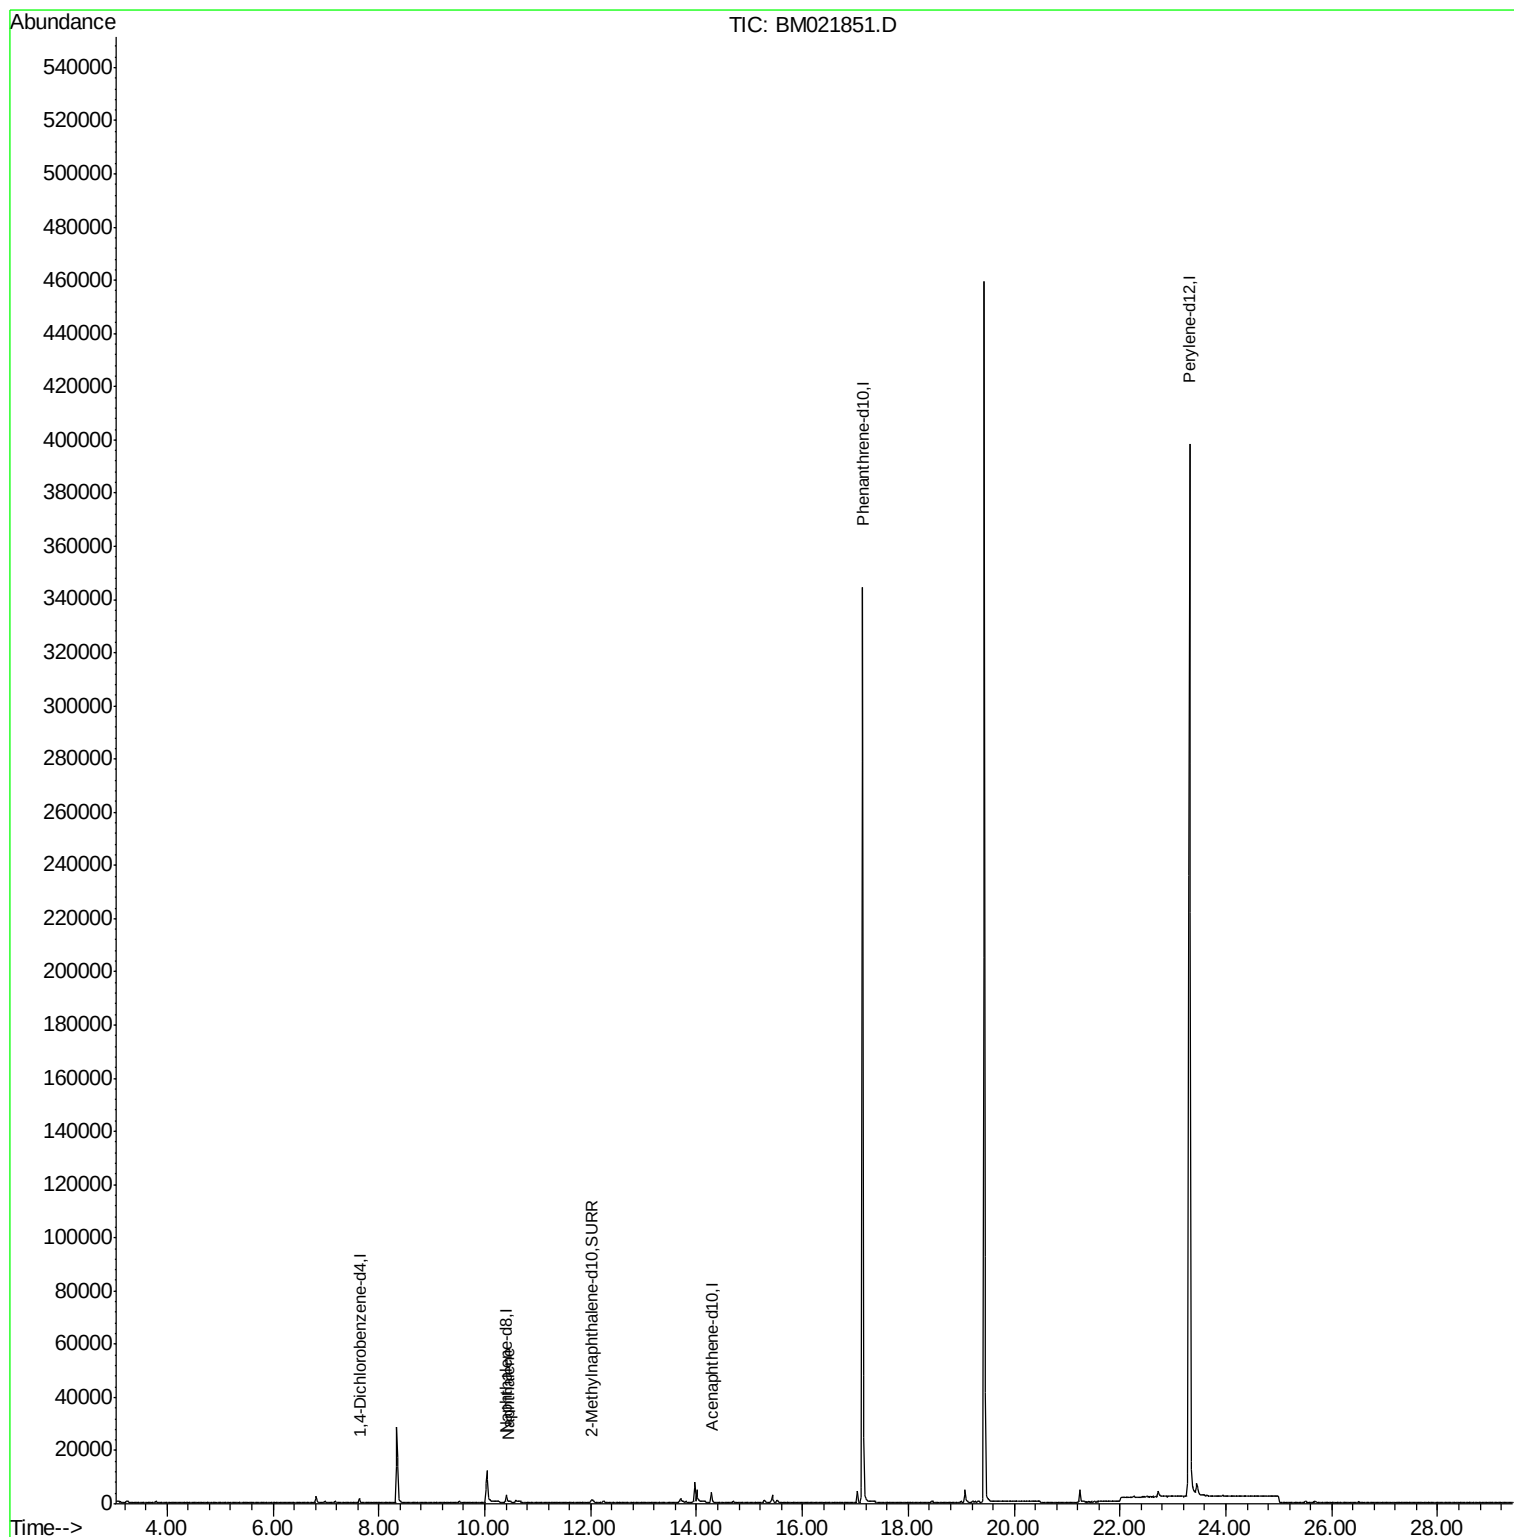

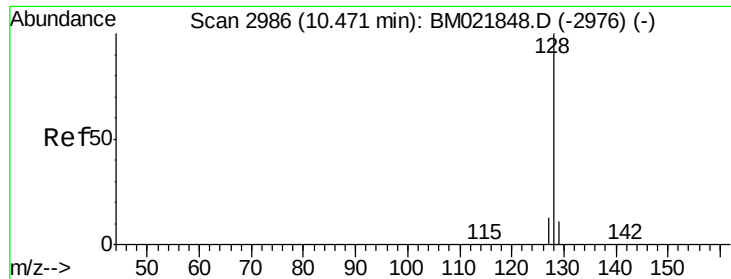

#3

Naphthalene

Concen: 0.024 ng/ul

RT: 10.46 min Scan# 2983

Delta R.T. -0.02 min

Lab File: BM021851.D

Acq: 05 Aug 2019 20:30

Instrument :

BNA_M

ClientSampleId :

A52N6


Tgt Ion:128 Resp: 235

Ion Ratio Lower Upper

128 100

129 39.2 12.3 18.5#

127 34.2 13.0 19.6#

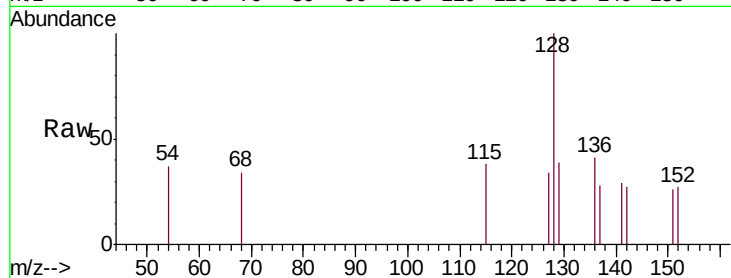

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

